
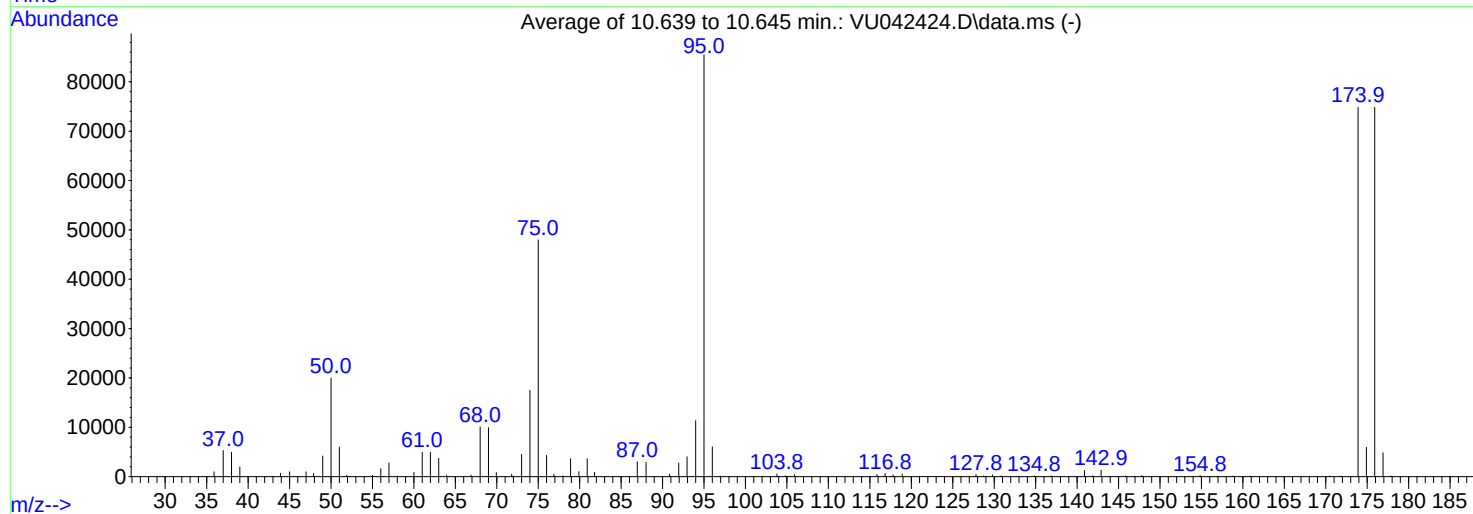


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022521\
Data File : VU042424.D
Acq On : 25 Feb 2021 09:16
Operator : SY/MD
Sample : BFB34
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB301

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM022521.M
Title : TRACE VOA SOM01.0
Last Update : Fri Feb 26 06:20:15 2021

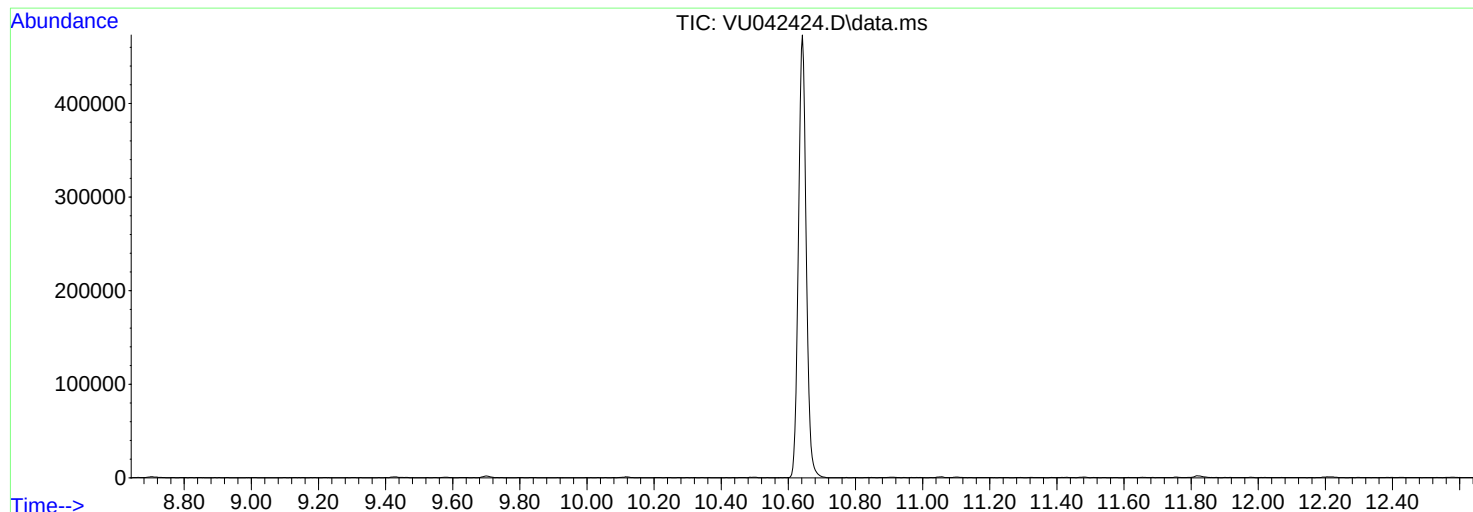

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.4	19968	PASS
75	95	30	80	56.1	47965	PASS
95	95	100	100	100.0	85464	PASS
96	95	5	9	7.1	6052	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	87.6	74837	PASS
175	174	5	9	7.9	5944	PASS
176	174	95	101	100.0	74829	PASS
177	176	5	9	6.5	4834	PASS

m/z	Abundance
35.90	1019.0
37.00	5343.0
38.00	5095.0
39.00	1963.0
40.00	147.0
42.90	129.0
43.90	882.0
45.00	1020.0
47.00	1036.0
47.90	667.0
49.00	4315.0
50.00	19832.0
51.00	6173.0
51.90	229.0
55.00	280.0
56.00	1678.0
57.00	2985.0
58.00	157.0
60.00	823.0
61.00	5072.0
62.00	5201.0
63.00	3748.0
64.00	331.0
66.90	350.0
68.00	10329.0
69.00	10073.0
69.90	886.0
71.80	501.0
73.00	4464.0
74.00	17688.0
75.00	48536.0
76.00	4533.0
76.90	530.0
77.90	241.0
78.90	3536.0
79.90	1020.0
80.90	3669.0
81.80	830.0
83.00	121.0
87.00	2895.0
88.00	2923.0
90.90	489.0
91.90	2943.0
93.00	3995.0
94.00	11366.0
95.00	85344.0
96.00	6176.0
97.00	112.0
103.80	582.0
104.80	131.0
105.90	342.0
115.90	405.0
116.80	572.0
117.80	313.0
118.90	477.0
127.80	393.0
128.70	170.0
129.80	357.0
130.90	156.0
134.90	189.0
136.80	155.0
140.90	1256.0
141.90	197.0
142.90	1395.0
145.90	145.0
147.80	245.0
154.80	225.0
158.80	156.0
160.90	140.0
170.40	126.0
171.70	275.0
173.90	73736.0
174.90	6008.0
175.90	72896.0
176.90	4783.0
177.90	158.0

Instrument :
MSVOA_U
ClientSampleId :
BFB301

m/z	Abundance
35.00	1000.0
37.00	5472.0
38.00	5122.0
39.00	1986.0
40.00	159.0
42.90	100.0
43.90	942.0
45.00	984.0
47.00	982.0
47.90	656.0
49.00	4314.0
50.00	20640.0
51.00	6229.0
51.90	240.0
55.00	267.0
56.00	1673.0
57.00	2870.0
58.00	146.0
60.00	908.0
61.00	5169.0
62.00	5154.0
63.00	3753.0
63.90	358.0
66.90	331.0
68.00	10467.0
69.00	10249.0
70.00	830.0
71.80	525.0
73.00	4675.0
74.00	18000.0
75.00	49536.0
76.00	4426.0
76.90	485.0
78.90	3725.0
79.90	1022.0
80.90	3687.0
81.80	911.0
86.90	3062.0
88.00	2970.0
90.90	528.0
92.00	2853.0
93.00	4203.0
94.00	11697.0
95.00	88216.0
96.00	6252.0
96.90	130.0
103.80	597.0
104.80	160.0
105.90	406.0
115.90	424.0
116.90	638.0
117.80	363.0
118.90	557.0
127.80	426.0
128.70	176.0
129.80	348.0
130.90	140.0
134.90	210.0
136.80	156.0
140.90	1323.0
141.90	198.0
142.90	1369.0
143.80	103.0
144.60	102.0
145.80	156.0
146.90	104.0
147.80	261.0
154.80	241.0
156.90	132.0
158.80	142.0
160.90	116.0
170.50	149.0
173.90	77416.0
174.90	6115.0
175.90	77536.0
176.90	5012.0
177.80	151.0

Instrument :
MSVOA_U
ClientSampleId :
BFB301

m/z	Abundance
35.90	885.0
37.00	5091.0
38.00	4618.0
39.00	1869.0
40.00	155.0
43.90	884.0
45.00	880.0
47.00	885.0
47.90	541.0
49.00	3964.0
50.00	19432.0
51.00	5640.0
51.90	284.0
55.00	215.0
56.00	1501.0
57.00	2553.0
58.00	125.0
60.00	876.0
61.00	4681.0
62.00	4582.0
63.00	3555.0
63.90	313.0
66.90	283.0
68.00	9428.0
69.00	9444.0
70.00	708.0
71.80	474.0
73.00	4389.0
74.00	16768.0
75.00	45824.0
76.00	3962.0
76.90	392.0
78.00	248.0
78.90	3588.0
79.90	945.0
80.90	3567.0
81.80	888.0
86.90	3065.0
88.00	2832.0
90.80	499.0
92.00	2481.0
92.90	3914.0
94.00	10977.0
95.00	82832.0
96.00	5727.0
96.90	127.0
103.80	488.0
104.80	162.0
105.90	432.0
115.80	399.0
116.90	631.0
117.80	415.0
118.90	594.0
127.80	423.0
128.80	140.0
129.80	358.0
130.80	126.0
134.80	224.0
136.90	149.0
140.90	1173.0
141.90	180.0
142.90	1209.0
143.90	126.0
145.80	138.0
146.90	105.0
147.80	213.0
149.90	111.0
154.90	215.0
156.90	148.0
158.80	106.0
170.60	130.0
171.90	280.0
173.90	73360.0
174.90	5710.0
175.90	74056.0
176.90	4707.0
177.80	125.0

Instrument :
MSVOA_U
ClientSampleId :
BFB301

m/z	Abundance
39.90	106.0
43.90	221.0

Instrument :
MSVOA_U
ClientSampleId :
BFB301