

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU022619\
 Data File : VU029672.D
 Acq On : 26 Feb 2019 10:37
 Operator : JC/SP
 Sample : VU0226WBL01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0226WBL01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U020519DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.694	494	499	509	rVB5	6830	11446	7.33%	2.151%
2	4.881	1170	1179	1183	rBV5	1191	1938	1.24%	0.364%
3	4.977	1206	1209	1219	rVB4	1331	1774	1.14%	0.333%
4	5.736	1432	1445	1465	rBV	72319	148456	95.06%	27.898%
5	5.894	1482	1494	1504	rVB5	1417	2599	1.66%	0.488%
6	7.482	1979	1988	1995	rBV3	1373	2496	1.60%	0.469%
7	8.180	2192	2205	2214	rBV2	1707	3352	2.15%	0.630%
8	8.389	2261	2270	2276	rBV6	1604	3023	1.94%	0.568%
9	9.382	2570	2579	2587	rBV4	1399	2357	1.51%	0.443%
10	10.308	2856	2867	2884	rBV2	64258	113863	72.91%	21.397%
11	10.607	2948	2960	2970	rBV4	11720	19597	12.55%	3.683%
12	10.778	3005	3013	3022	rBV4	2132	3249	2.08%	0.611%
13	11.099	3102	3113	3121	rBV4	1387	2678	1.71%	0.503%
14	11.324	3173	3183	3190	rBV4	1610	2674	1.71%	0.503%
15	11.424	3212	3214	3223	rVB4	1736	1926	1.23%	0.362%
16	11.488	3223	3234	3235	rBV4	4127	5146	3.30%	0.967%
17	11.861	3335	3350	3375	rBV	82067	156175	100.00%	29.349%
18	12.482	3531	3543	3554	rBV	12532	20952	13.42%	3.937%
19	13.514	3853	3864	3873	rBV5	3490	6480	4.15%	1.218%
20	13.691	3913	3919	3925	rBV5	1426	1622	1.04%	0.305%
21	13.755	3930	3939	3940	rBV4	2610	2769	1.77%	0.520%
22	13.996	4004	4014	4022	rBV4	4752	8571	5.49%	1.611%
23	14.276	4093	4101	4112	rVB	4186	5999	3.84%	1.127%
24	15.880	4596	4600	4609	rVB6	2354	2991	1.92%	0.562%


Sum of corrected areas: 532133

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU022619\
Data File : VU029672.D
Acq On : 26 Feb 2019 10:37
Operator : JC/SP
Sample : VU0226WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0226WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U020519DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

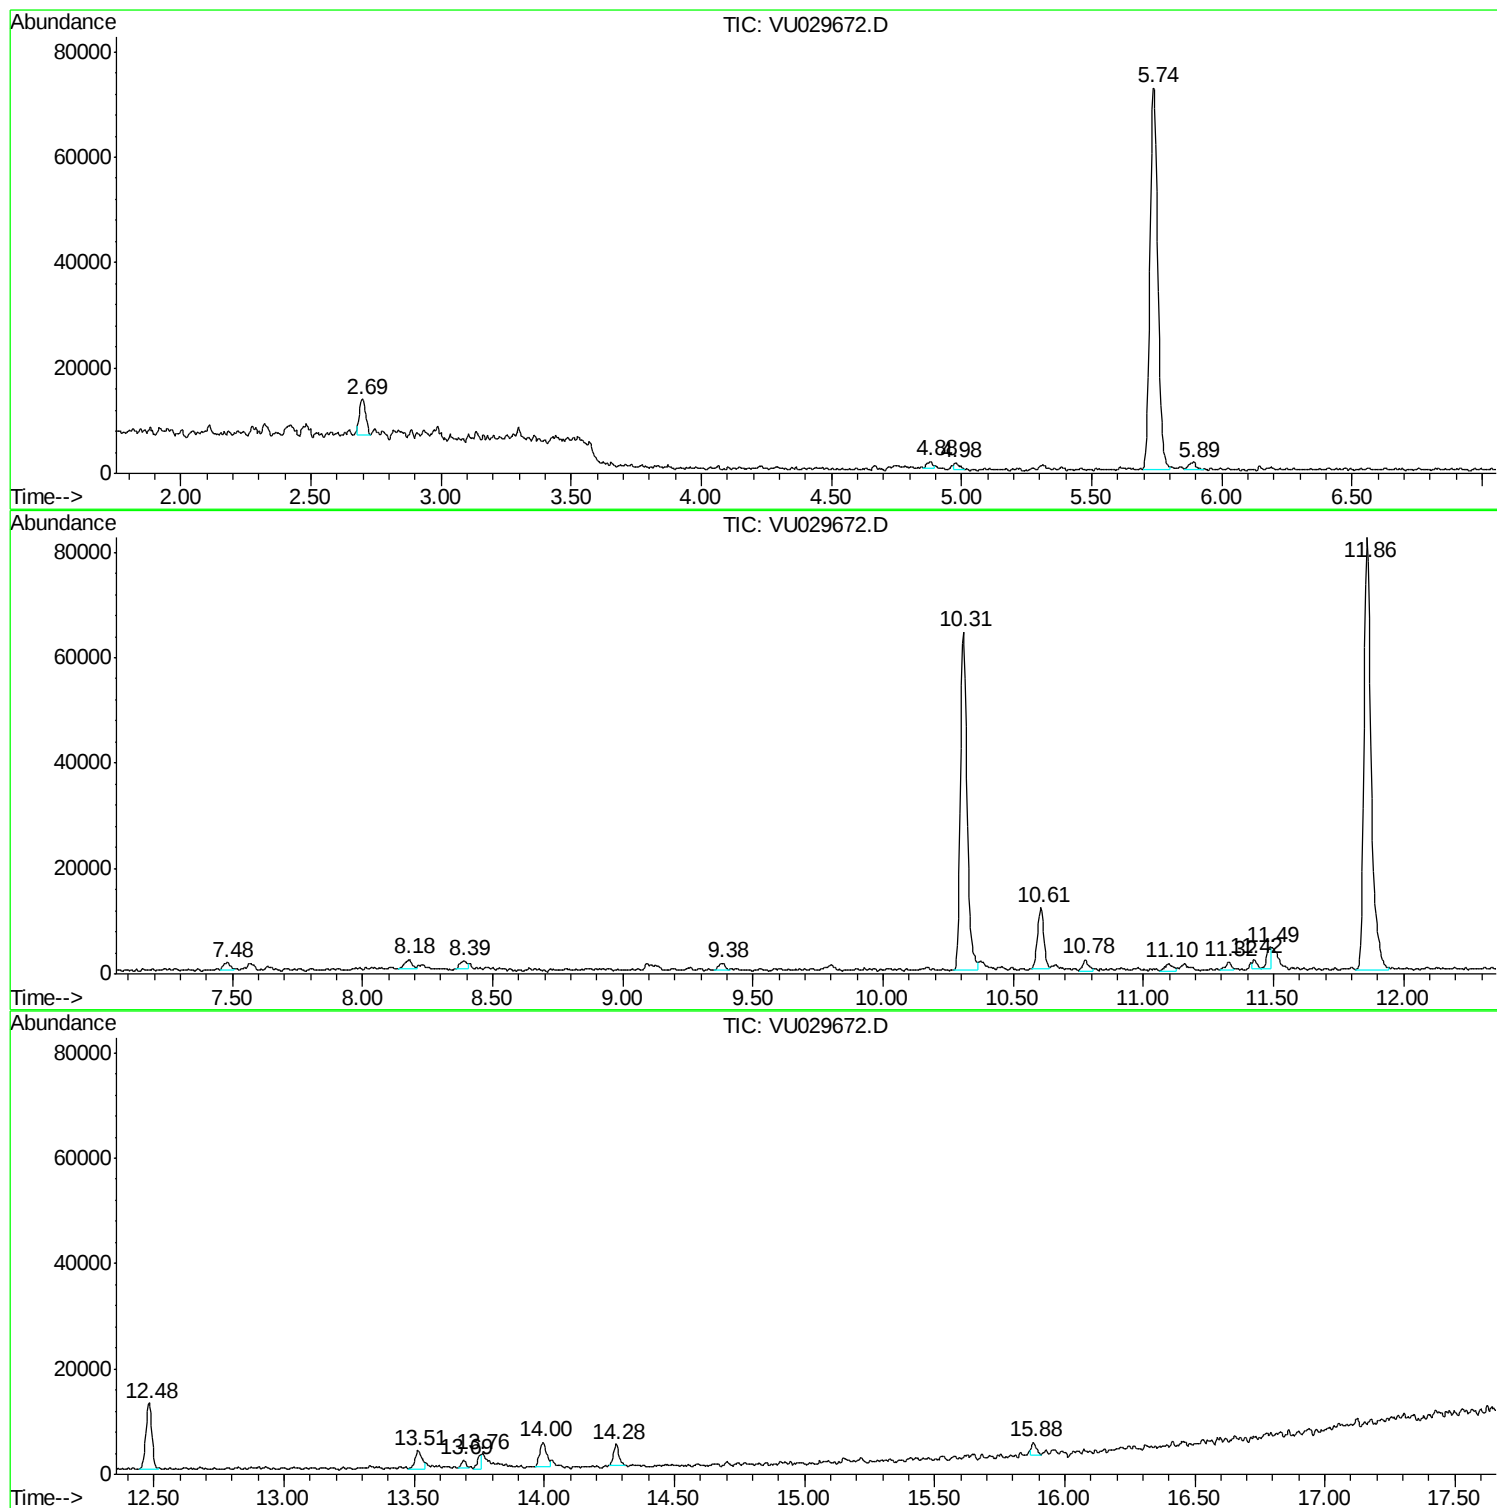

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU022619\
Data File : VU029672.D
Acq On : 26 Feb 2019 10:37
Operator : JC/SP
Sample : VU0226WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0226WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U020519DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU022619\
Data File : VU029672.D
Acq On : 26 Feb 2019 10:37
Operator : JC/SP
Sample : VU0226WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0226WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U020519DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc