


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU022619\
 Data File : VU029670.D
 Acq On : 26 Feb 2019 09:19
 Operator : JC/SP
 Sample : BFB
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U020519DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Fri Feb 08 10:52:46 2019

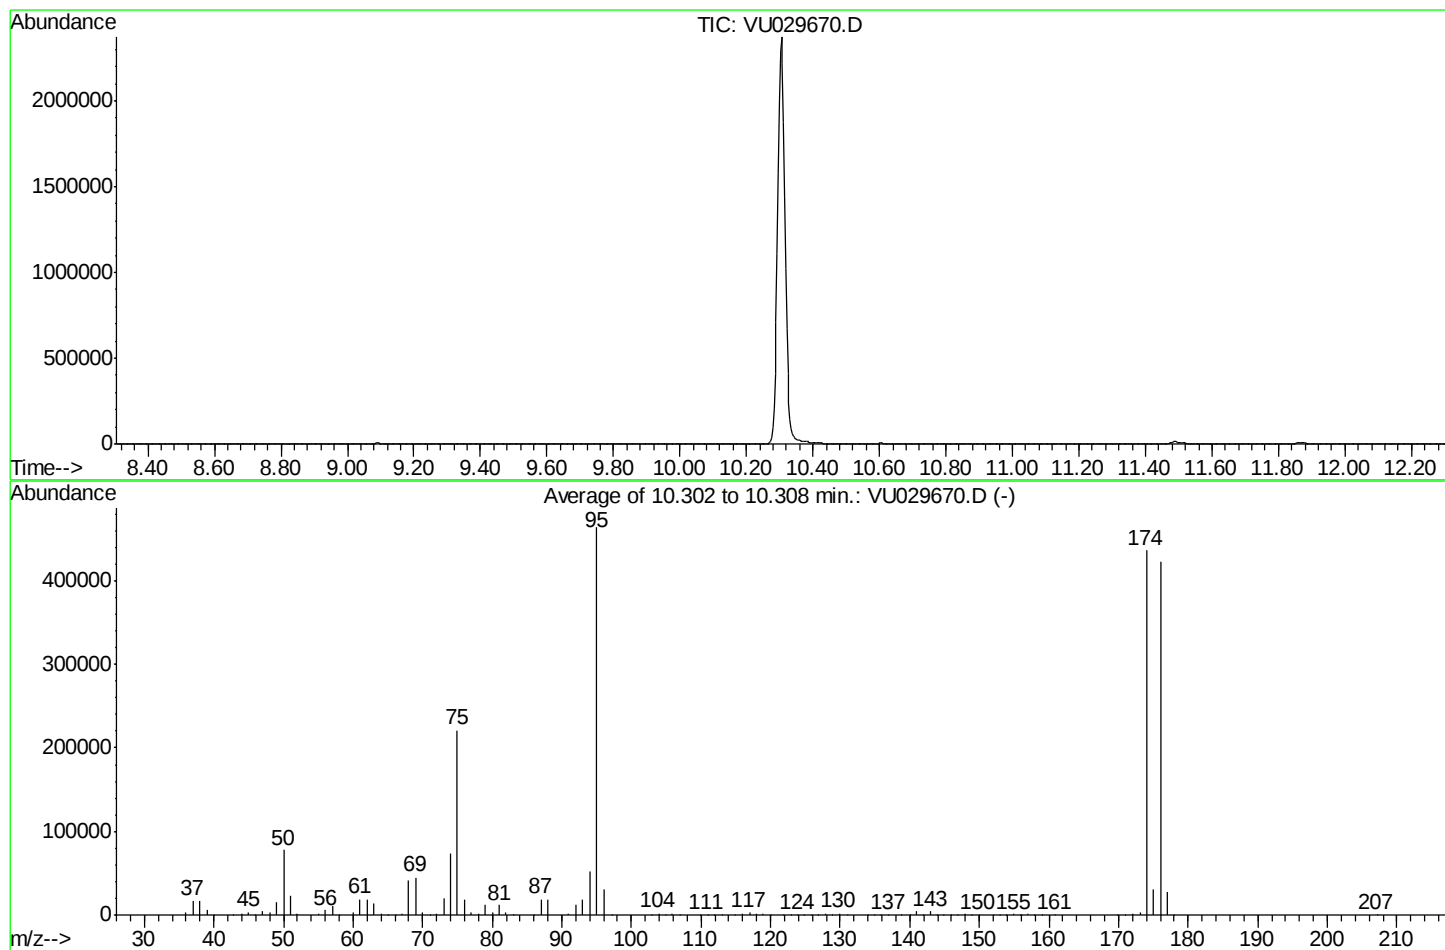

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2851

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	77837	PASS
75	95	30	60	47.6	220736	PASS
95	95	100	100	100.0	463914	PASS
96	95	5	9	6.5	30333	PASS
173	174	0.00	2	0.9	3812	PASS
174	95	50	100	94.0	436010	PASS
175	174	5	9	7.2	31282	PASS
176	174	95	101	96.8	422229	PASS
177	176	5	9	6.5	27306	PASS