

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU022620\
 Data File : VU036915.D
 Acq On : 26 Feb 2020 15:17
 Operator : JC/MD
 Sample : L1687-05 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AS5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.614	78	85	99	rBV	141160	151139	14.74%	1.964%
2	1.929	175	183	197	rVB	120640	158935	15.50%	2.065%
3	2.591	377	389	405	rBV	202691	334025	32.58%	4.340%
4	2.726	428	431	432	rBV2	330	171	0.02%	0.002%
5	2.749	436	438	442	rVB2	199	119	0.01%	0.002%
6	2.784	443	449	450	rBV	402	376	0.04%	0.005%
7	3.080	534	541	547	rBV4	838	1240	0.12%	0.016%
8	3.122	552	554	555	rBV	186	81	0.01%	0.001%
9	3.221	575	585	600	rVB	4463	9458	0.92%	0.123%
10	3.282	601	604	609	rBV	226	198	0.02%	0.003%
11	3.324	614	617	623	rBB2	168	175	0.02%	0.002%
12	3.385	633	636	640	rBV	120	139	0.01%	0.002%
13	3.453	654	657	661	rBV2	160	146	0.01%	0.002%
14	3.479	661	665	668	rBV	213	171	0.02%	0.002%
15	3.498	668	671	676	rVB	243	191	0.02%	0.002%
16	3.530	676	681	682	rBV	260	228	0.02%	0.003%
17	3.591	697	700	703	rBV	189	100	0.01%	0.001%
18	3.610	703	706	710	rVV	236	210	0.02%	0.003%
19	3.643	714	716	718	rVB	232	91	0.01%	0.001%
20	3.672	721	725	727	rBV2	267	207	0.02%	0.003%
21	3.688	727	730	734	rVV2	251	223	0.02%	0.003%
22	3.713	735	738	743	rVV2	224	236	0.02%	0.003%
23	3.739	744	746	747	rVB2	317	93	0.01%	0.001%
24	3.755	749	751	755	rBV	145	85	0.01%	0.001%
25	3.848	776	780	785	rBV2	195	186	0.02%	0.002%
26	3.893	791	794	797	rBV	234	142	0.01%	0.002%
27	3.958	811	814	817	rBV2	185	128	0.01%	0.002%
28	4.102	855	859	861	rBV	179	119	0.01%	0.002%
29	4.157	874	876	880	rVB	226	119	0.01%	0.002%
30	4.183	880	884	889	rBV2	164	155	0.02%	0.002%
31	4.292	915	918	922	rVV2	190	155	0.02%	0.002%
32	4.315	922	925	928	rVB	213	106	0.01%	0.001%
33	4.430	958	961	965	rVV	192	149	0.01%	0.002%
34	4.459	965	970	973	rVV2	221	227	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU022620\
 Data File : VU036915.D
 Acq On : 26 Feb 2020 15:17
 Operator : JC/MD
 Sample : L1687-05 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AS5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
 Title : VOC Analysis

35	4.504	982	984	987	rVB2	174	101	0.01%	0.001%
36	4.533	990	993	997	rVB2	188	141	0.01%	0.002%
37	4.556	997	1000	1005	rVB	254	210	0.02%	0.003%
38	4.601	1012	1014	1018	rVB	239	133	0.01%	0.002%
39	4.671	1018	1036	1067	rBV	110081	260247	25.39%	3.381%
40	5.016	1140	1143	1145	rBV2	259	174	0.02%	0.002%
41	5.106	1153	1171	1194	rBV	179471	386778	37.73%	5.025%
42	5.376	1252	1255	1257	rVB	202	105	0.01%	0.001%
43	5.411	1261	1266	1272	rBV3	542	766	0.07%	0.010%
44	5.475	1283	1286	1288	rBV	178	83	0.01%	0.001%
45	5.527	1299	1302	1307	rVB2	204	228	0.02%	0.003%
46	5.610	1325	1328	1331	rBV2	181	142	0.01%	0.002%
47	5.678	1346	1349	1354	rBV2	165	181	0.02%	0.002%
48	5.761	1354	1375	1394	rBV2	393307	1025143	100.00%	13.320%
49	6.070	1468	1471	1477	rVB2	324	286	0.03%	0.004%
50	6.141	1490	1493	1495	rBV2	381	181	0.02%	0.002%
51	6.282	1522	1537	1556	rVV	327121	607967	59.31%	7.899%
52	6.565	1616	1625	1635	rVB8	2826	5003	0.49%	0.065%
53	6.639	1645	1648	1651	rBV	195	115	0.01%	0.001%
54	6.726	1660	1675	1697	rBV	242667	468061	45.66%	6.082%
55	6.803	1697	1699	1702	rVB	321	152	0.01%	0.002%
56	6.858	1714	1716	1720	rVB2	523	271	0.03%	0.004%
57	6.887	1720	1725	1728	rBV	161	149	0.01%	0.002%
58	6.935	1736	1740	1743	rBV	149	132	0.01%	0.002%
59	6.970	1748	1751	1754	rBV2	198	120	0.01%	0.002%
60	7.051	1773	1776	1781	rBV	110	102	0.01%	0.001%
61	7.205	1821	1824	1825	rBV	245	157	0.02%	0.002%
62	7.305	1852	1855	1857	rBV2	165	95	0.01%	0.001%
63	7.340	1864	1866	1869	rVV2	133	98	0.01%	0.001%
64	7.411	1885	1888	1894	rVB	117	111	0.01%	0.001%
65	7.504	1913	1917	1919	rBV	194	94	0.01%	0.001%
66	7.527	1919	1924	1926	rBV	160	121	0.01%	0.002%
67	7.594	1930	1945	1965	rBV	132382	230450	22.48%	2.994%
68	7.752	1991	1994	1995	rBV	211	127	0.01%	0.002%
69	7.855	2024	2026	2029	rBV2	145	86	0.01%	0.001%
70	7.925	2034	2048	2065	rBV	477647	816736	79.67%	10.612%
71	8.138	2113	2114	2117	rVB	150	80	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU022620\
 Data File : VU036915.D
 Acq On : 26 Feb 2020 15:17
 Operator : JC/MD
 Sample : L1687-05 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AS5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
 Title : VOC Analysis

72	8.163	2118	2122	2123	rBV	175	130	0.01%	0.002%
73	8.205	2123	2135	2157	rVV2	91927	153678	14.99%	1.997%
74	8.392	2190	2193	2198	rBV	124	114	0.01%	0.001%
75	8.572	2245	2249	2252	rBV2	423	290	0.03%	0.004%
76	8.662	2263	2277	2313	rBV	309772	584270	56.99%	7.592%
77	8.864	2338	2340	2343	rBV	169	79	0.01%	0.001%
78	8.896	2347	2350	2351	rBV	200	92	0.01%	0.001%
79	8.935	2361	2362	2367	rVB2	135	108	0.01%	0.001%
80	9.019	2383	2388	2389	rBV	145	89	0.01%	0.001%
81	9.044	2394	2396	2402	rVB	182	128	0.01%	0.002%
82	9.102	2410	2414	2417	rBV	132	109	0.01%	0.001%
83	9.205	2442	2446	2448	rBV	202	129	0.01%	0.002%
84	9.263	2460	2464	2468	rBV2	157	179	0.02%	0.002%
85	9.440	2506	2519	2553	rBV	448899	748997	73.06%	9.732%
86	9.588	2562	2565	2571	rBV2	339	299	0.03%	0.004%
87	9.620	2572	2575	2577	rVV	153	93	0.01%	0.001%
88	9.916	2662	2667	2671	rBV2	275	364	0.04%	0.005%
89	9.961	2678	2681	2683	rBV2	231	174	0.02%	0.002%
90	10.031	2701	2703	2705	rBV	231	94	0.01%	0.001%
91	10.491	2844	2846	2850	rVB	220	103	0.01%	0.001%
92	10.533	2856	2859	2860	rBV	188	90	0.01%	0.001%
93	10.774	2922	2934	2952	rVB	312297	506447	49.40%	6.580%
94	11.019	3007	3010	3012	rBV2	232	183	0.02%	0.002%
95	11.096	3029	3034	3037	rBV	309	321	0.03%	0.004%
96	11.340	3106	3110	3113	rBV	236	209	0.02%	0.003%
97	11.359	3113	3116	3118	rVV	191	110	0.01%	0.001%
98	11.662	3205	3210	3215	rBV	262	299	0.03%	0.004%
99	11.829	3250	3262	3279	rVB	367029	598663	58.40%	7.779%
100	12.211	3368	3381	3396	rBV	389523	635834	62.02%	8.262%


Sum of corrected areas: 7696324

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU022620\
Data File : VU036915.D
Acq On : 26 Feb 2020 15:17
Operator : JC/MD
Sample : L1687-05 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AS5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

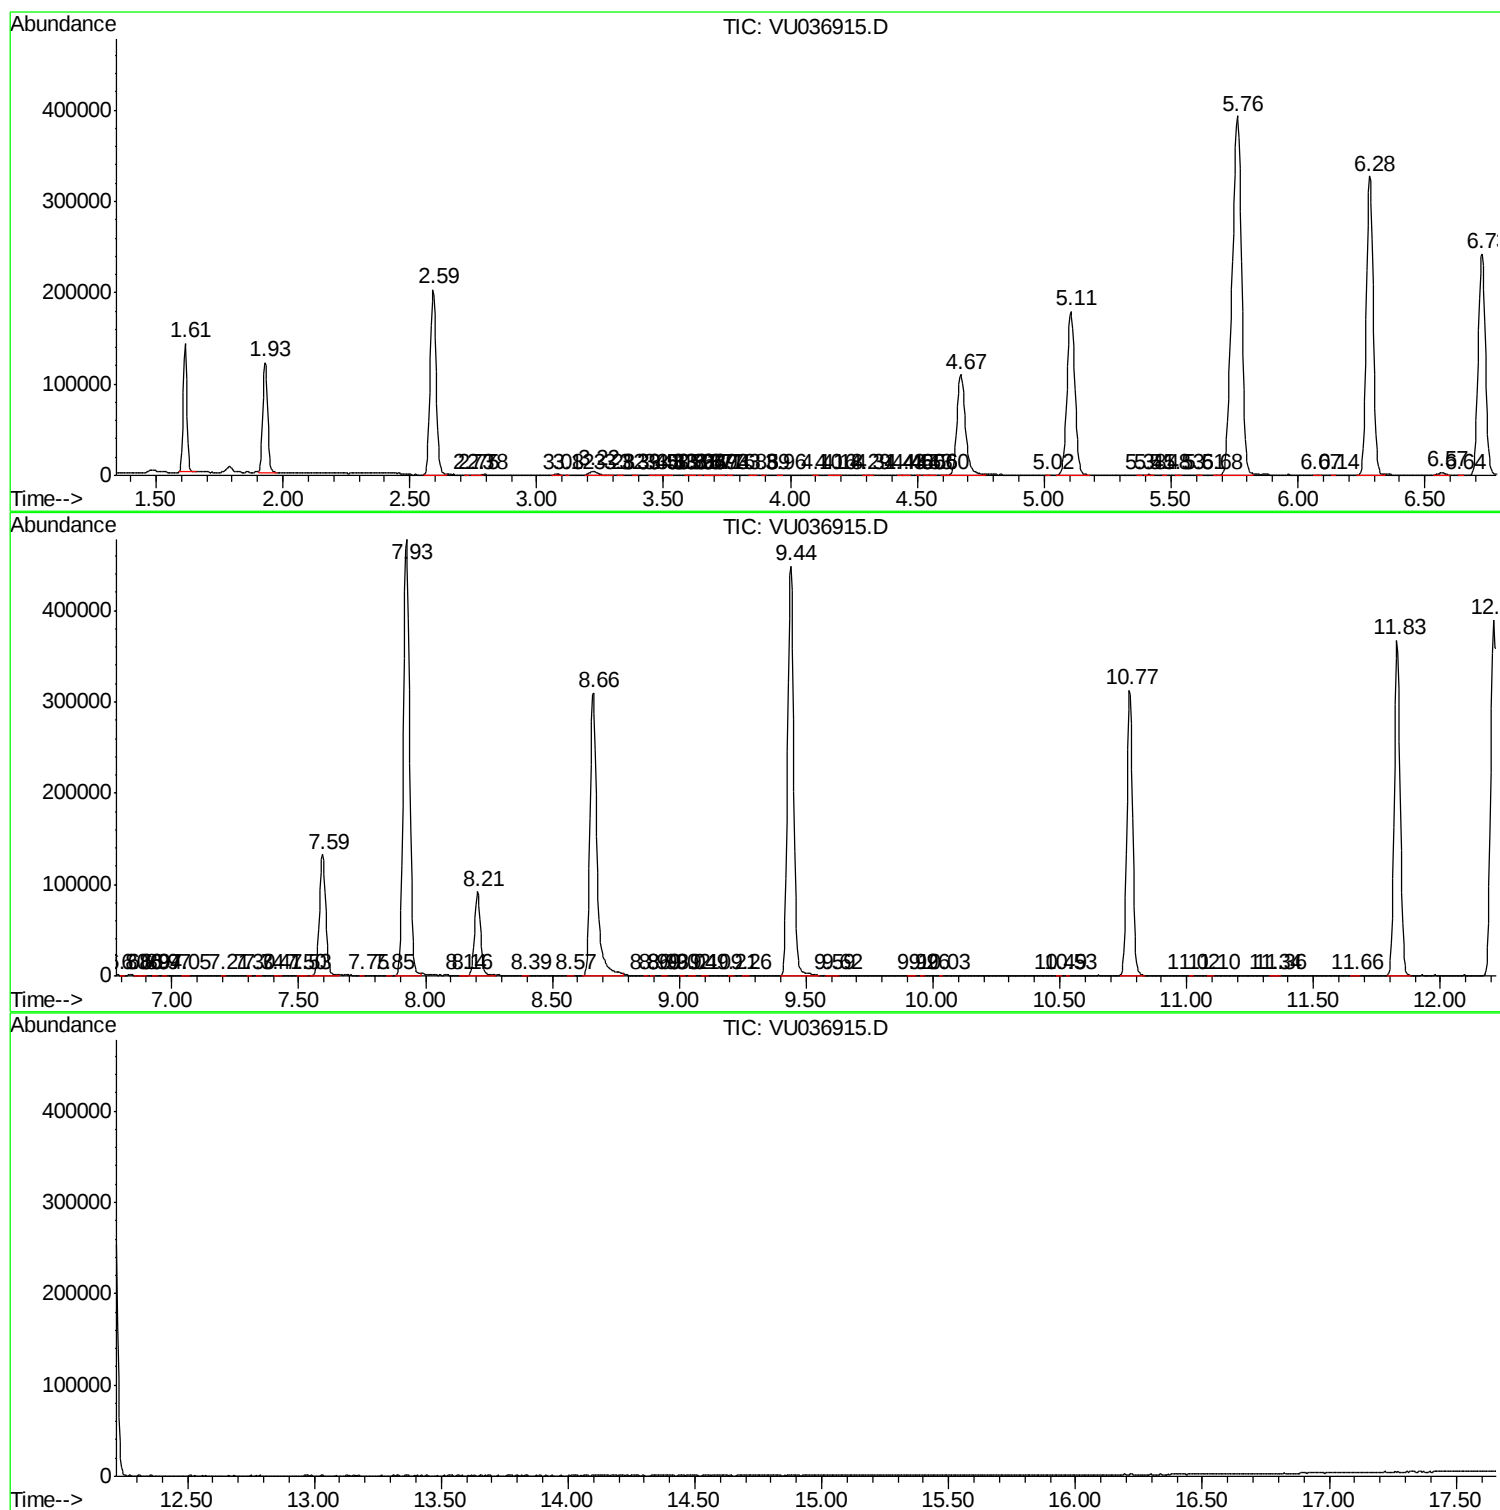

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU022620\
Data File : VU036915.D
Acq On : 26 Feb 2020 15:17
Operator : JC/MD
Sample : L1687-05 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AS5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU022620\
Data File : VU036915.D
Acq On : 26 Feb 2020 15:17
Operator : JC/MD
Sample : L1687-05 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AS5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc