


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU022620\
 Data File : VU036907.D
 Acq On : 26 Feb 2020 09:44
 Operator : JC/MD
 Sample : BFB52
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB52

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
 Title : VOC Analysis
 Last Update : Thu Feb 27 04:47:27 2020

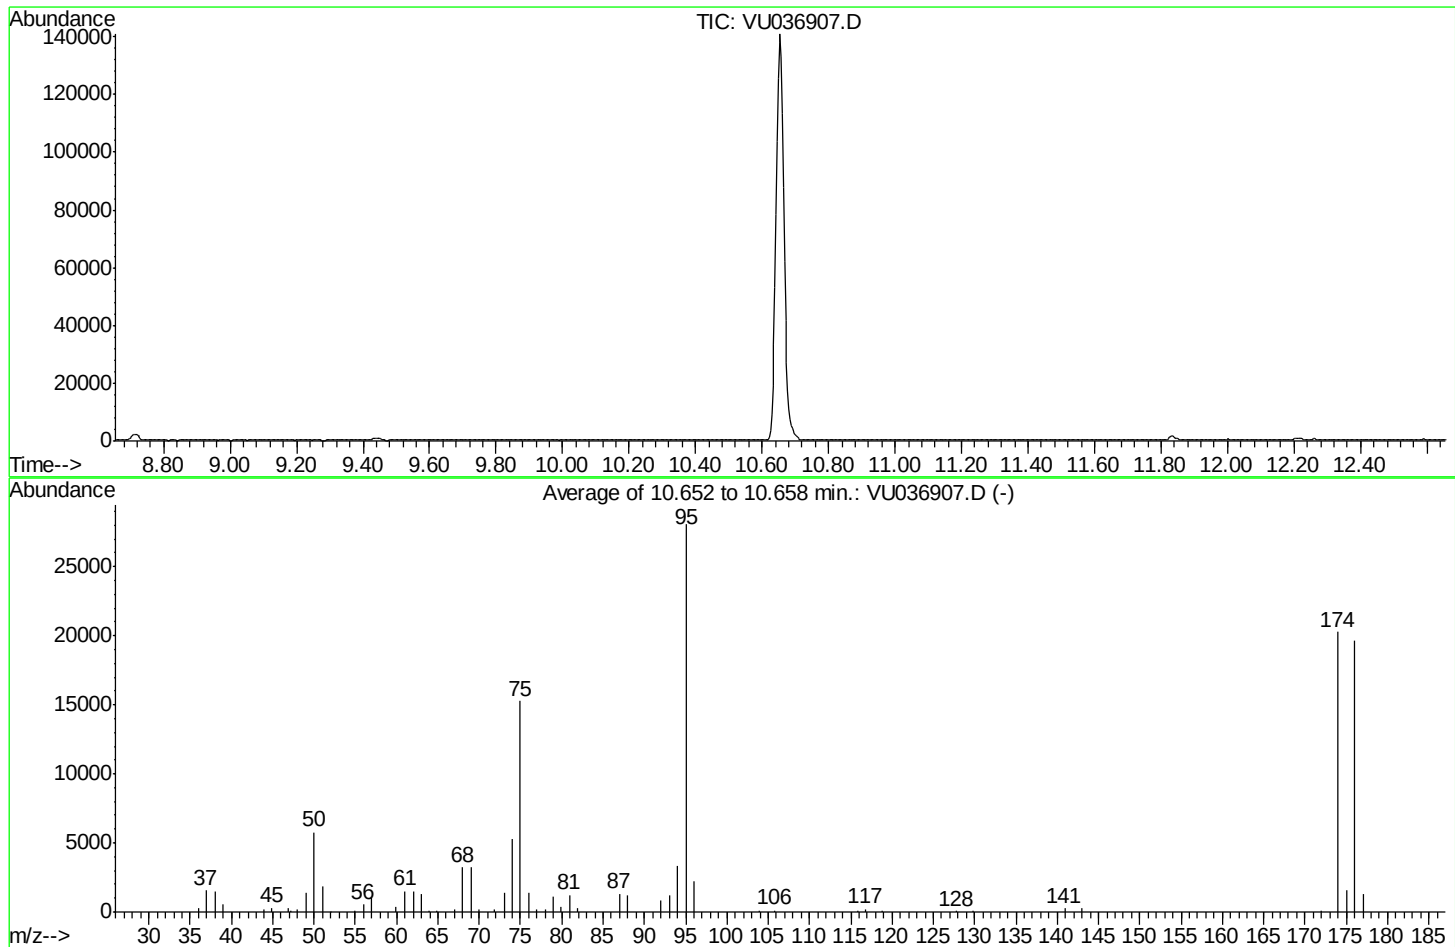

AutoFind: Scans 2896, 2897, 2898; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	5793	PASS
75	95	30	80	54.4	15275	PASS
95	95	100	100	100.0	28061	PASS
96	95	5	9	8.0	2251	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.3	20282	PASS
175	174	5	9	8.0	1613	PASS
176	174	95	101	97.0	19666	PASS
177	176	5	9	6.4	1261	PASS

m/z	Abundance
36.00	270.0
37.00	1650.0
38.00	1587.0
38.90	524.0
43.90	512.0
44.90	316.0
46.90	285.0
47.20	295.0
47.90	217.0
49.00	1388.0
50.00	5865.0
51.00	1866.0
54.90	123.0
56.00	579.0
57.00	1021.0
59.90	321.0
61.00	1640.0
62.00	1468.0
63.00	1344.0
63.90	135.0
64.90	150.0
67.00	146.0
68.00	3323.0
69.00	3259.0
70.00	222.0
71.80	190.0
73.00	1447.0
74.00	5430.0
75.00	15330.0
76.00	1421.0
76.90	186.0
77.90	144.0
79.00	1139.0
79.90	427.0
80.90	1256.0
81.90	292.0
87.00	1331.0
88.00	1222.0
92.10	894.0
93.00	1185.0
94.00	3426.0
95.10	28176.0
96.00	2350.0
105.80	133.0
115.90	169.0
116.80	195.0
118.80	123.0
127.80	138.0
140.90	305.0
142.90	223.0
172.10	115.0
174.00	20136.0
175.00	1609.0
176.00	19328.0
177.00	1199.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

m/z	Abundance
35.90	320.0
36.90	1479.0
38.00	1411.0
38.90	579.0
43.90	501.0
44.90	287.0
46.90	325.0
48.00	199.0
49.10	1396.0
50.00	5537.0
51.00	1888.0
52.00	117.0
56.00	437.0
57.00	1005.0
59.90	331.0
61.00	1384.0
62.00	1483.0
63.00	1128.0
63.90	138.0
64.90	123.0
67.10	149.0
68.00	3020.0
69.00	3147.0
70.00	217.0
71.90	195.0
73.00	1358.0
74.00	5071.0
75.00	14802.0
76.00	1243.0
76.90	170.0
78.00	173.0
79.00	1005.0
79.90	340.0
80.90	1166.0
81.90	239.0
87.00	1278.0
88.00	1162.0
92.00	818.0
93.00	1110.0
94.00	3129.0
95.10	27304.0
96.00	2089.0
103.90	107.0
105.80	132.0
115.90	104.0
116.90	184.0
118.90	139.0
129.80	112.0
141.00	240.0
142.90	255.0
171.90	155.0
174.00	19808.0
175.00	1596.0
176.00	19424.0
177.00	1305.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

m/z	Abundance
36.00	334.0
37.00	1561.0
38.00	1585.0
38.90	591.0
43.90	492.0
44.90	305.0
46.90	337.0
48.00	209.0
49.00	1436.0
50.00	5979.0
51.00	1953.0
54.90	102.0
56.00	536.0
57.00	1032.0
59.90	336.0
61.00	1529.0
62.00	1534.0
63.00	1332.0
63.90	143.0
64.90	141.0
67.00	163.0
68.00	3378.0
69.00	3309.0
70.00	217.0
71.80	205.0
73.00	1455.0
74.00	5443.0
75.00	15694.0
76.00	1407.0
76.90	184.0
77.90	170.0
79.00	1120.0
79.90	403.0
80.90	1269.0
81.90	274.0
87.00	1324.0
88.00	1220.0
92.10	872.0
93.00	1241.0
94.00	3412.0
95.10	28704.0
96.00	2315.0
103.90	103.0
105.80	148.0
115.90	143.0
116.90	223.0
118.90	131.0
127.80	105.0
129.80	117.0
140.90	267.0
142.90	240.0
172.10	133.0
174.00	20904.0
175.00	1636.0
176.00	20248.0
177.00	1279.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

Scan 2884 (10.613 min): VU036907.D
BFB52

m/z	Abundance
39.80	133.0
43.90	340.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52