

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022621\
 Data File : VU042439.D
 Acq On : 26 Feb 2021 09:55
 Operator : SY/MD
 Sample : VU0226WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK205

Quant Time: Feb 26 21:52:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM022521.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Feb 26 21:52:13 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.225	114	4083	0.50	ug/L	0.00
5) Chlorobenzene-d5	9.361	117	3656	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.759	152	1956	0.50	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.606	65	1703	0.53	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	106.00%
4) 1,2-Dichloroethane-d4	5.680	65	1949	0.47	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	94.00%
7) 1,2-Dichloropropane-d6	6.658	67	1754	0.54	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	108.00%
8) Toluene-d8	7.845	98	4583	0.50	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	100.00%
10) 1,1,2,2-Tetrachloroeth...	10.696	84	1465	0.54	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	108.00%


Target Compounds						Qvalue
13) 1,2-Dibromo-3-chloropr...	12.701	75	9	0.02	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022621\
Data File : VU042439.D
Acq On : 26 Feb 2021 09:55
Operator : SY/MD
Sample : VU0226WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK205


Quant Time: Feb 26 21:52:37 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM022521.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Feb 26 21:52:13 2021
Response via : Initial Calibration

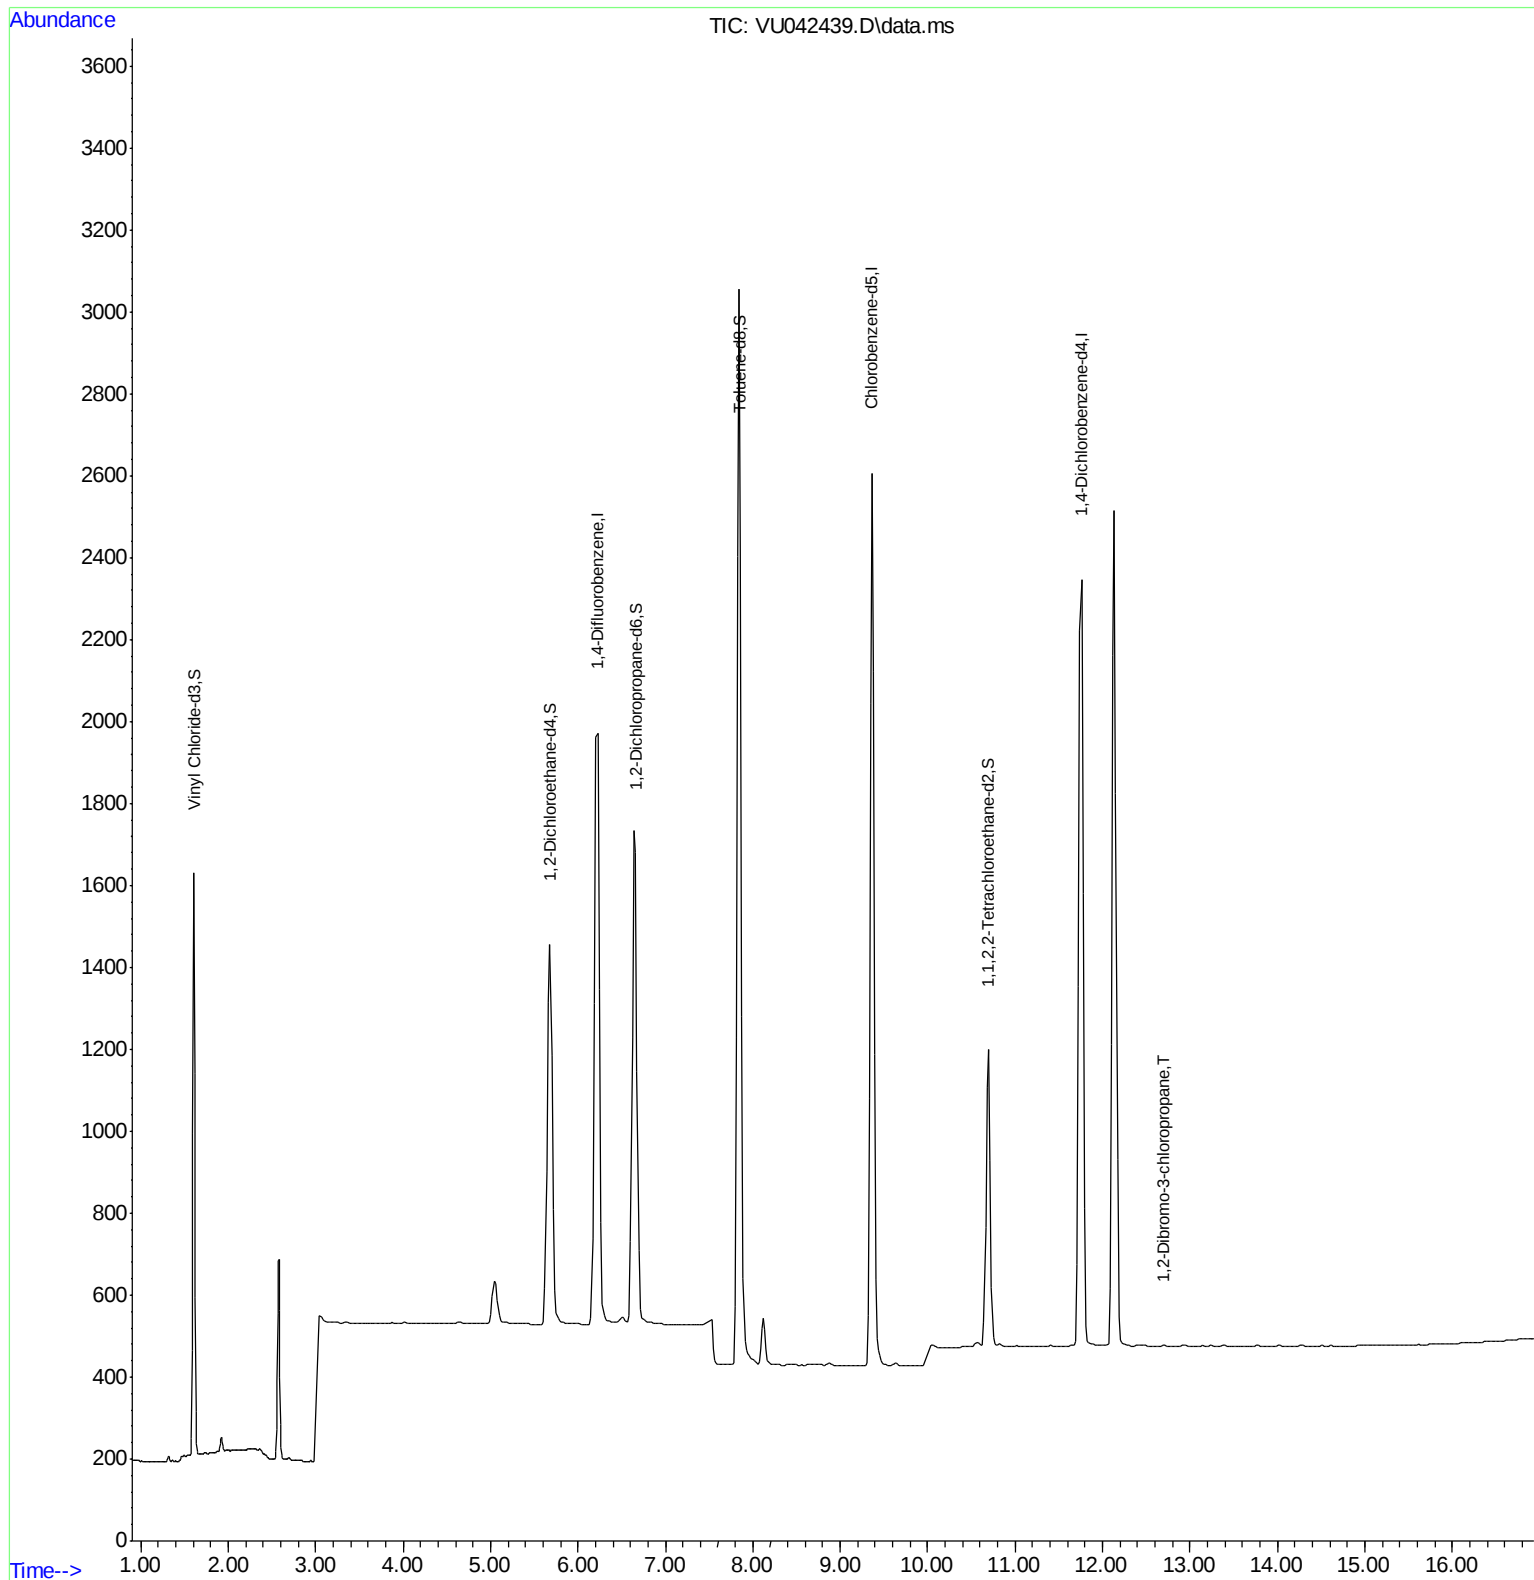

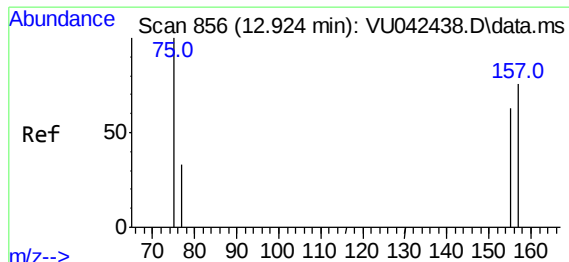

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.02 ug/L
 RT: 12.701 min Scan# 843
 Delta R.T. -0.223 min
 Lab File: VU042439.D
 Acq: 26 Feb 2021 09:55

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK205

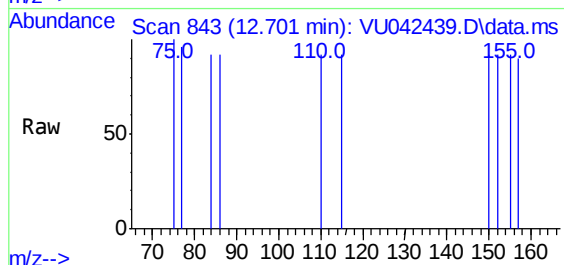

Tgt Ion: 75 Resp: 9

Ion	Ratio	Lower	Upper
75	100		
157	90.2	70.2	105.2
155	92.2	63.0	94.4

