
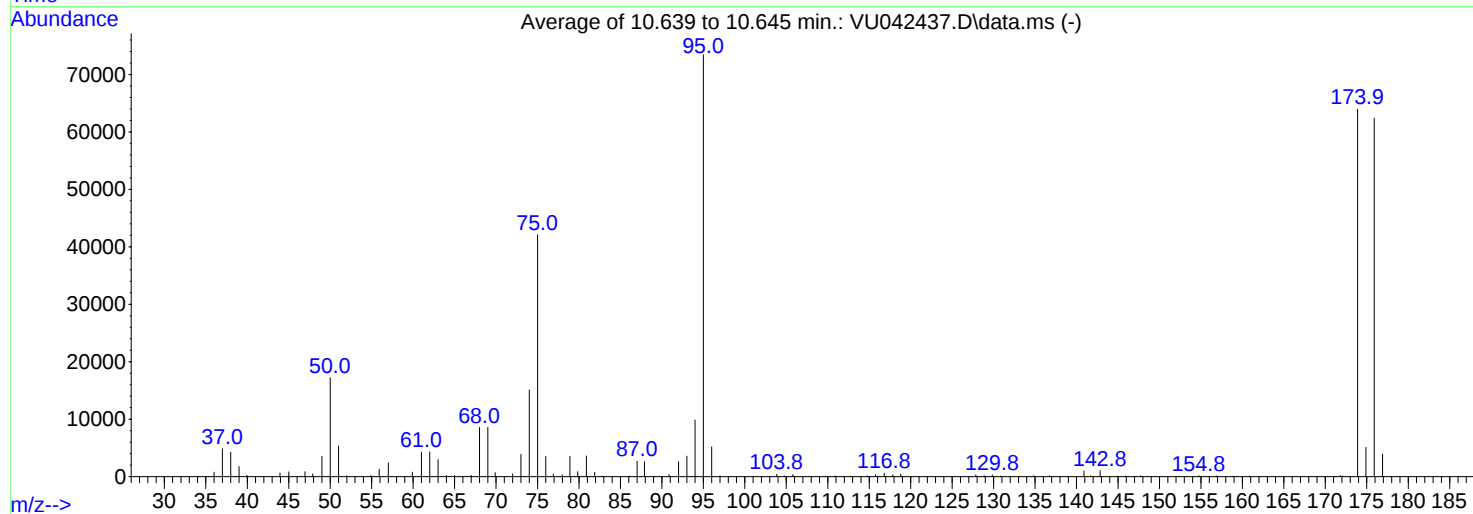


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022621\
Data File : VU042437.D
Acq On : 26 Feb 2021 08:45
Operator : SY/MD
Sample : BFB35
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB302

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM022521.M
Title : TRACE VOA SOM01.0
Last Update : Fri Feb 26 21:52:13 2021

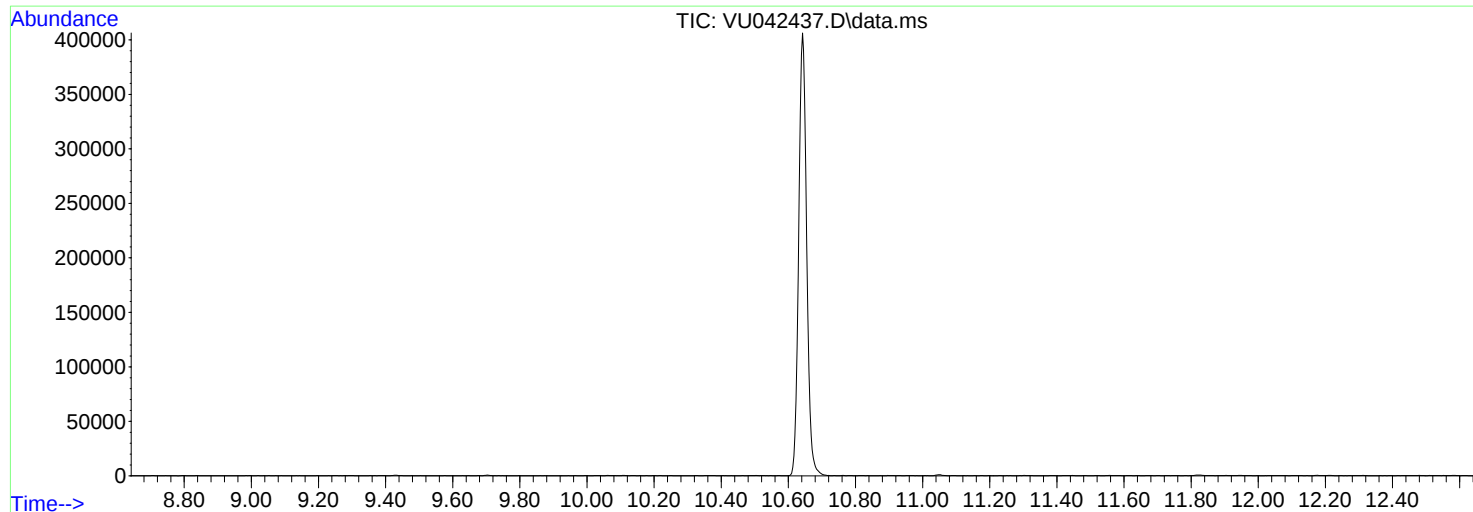

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.4	17211	PASS
75	95	30	80	57.4	42115	PASS
95	95	100	100	100.0	73419	PASS
96	95	5	9	7.1	5185	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	87.1	63979	PASS
175	174	5	9	8.0	5097	PASS
176	174	95	101	97.5	62387	PASS
177	176	5	9	6.3	3911	PASS

m/z	Abundance
36.00	817.0
37.00	4801.0
38.00	4162.0
39.00	1736.0
40.00	204.0
44.00	832.0
45.00	833.0
46.90	832.0
47.90	458.0
49.00	3608.0
50.00	16904.0
51.00	5530.0
51.90	158.0
54.90	209.0
55.90	1263.0
57.00	2387.0
59.90	716.0
61.00	4375.0
62.00	4220.0
63.00	3109.0
64.00	231.0
65.00	199.0
67.00	178.0
68.00	8627.0
69.00	8679.0
69.90	704.0
72.00	456.0
73.00	3912.0
74.00	15205.0
75.00	41536.0
76.00	3609.0
76.90	447.0
78.00	310.0
78.90	3529.0
79.80	825.0
80.90	3493.0
81.90	666.0
82.80	113.0
87.00	2481.0
87.90	2562.0
91.00	317.0
92.00	2528.0
93.00	3499.0
94.00	9492.0
95.00	72072.0
96.00	5287.0
97.00	157.0
103.80	398.0
104.70	156.0
105.80	401.0
110.90	127.0
112.70	115.0
114.70	131.0
115.80	303.0
116.80	669.0
117.90	334.0
118.80	447.0
127.90	274.0
128.90	128.0
129.80	287.0
130.80	106.0
134.90	180.0
136.80	150.0
140.90	978.0
141.70	166.0
142.80	1000.0
144.80	116.0
145.90	121.0
147.70	143.0
154.80	179.0
156.80	160.0
160.90	111.0
172.10	324.0
173.90	61672.0
174.90	5104.0
175.90	59768.0
176.90	3634.0

Instrument :
MSVOA_U
ClientSampleId :
BFB302

m/z	Abundance
36.00	831.0
37.00	4962.0
38.00	4352.0
39.00	1786.0
39.90	235.0
44.00	886.0
45.00	866.0
47.00	902.0
47.90	491.0
49.00	3633.0
50.00	17872.0
51.00	5536.0
51.90	173.0
54.90	202.0
55.90	1337.0
57.00	2446.0
59.90	834.0
61.00	4376.0
62.00	4424.0
63.00	3051.0
64.00	229.0
65.00	199.0
67.00	232.0
68.00	8845.0
69.00	8888.0
69.90	701.0
72.00	485.0
73.00	3988.0
74.00	15528.0
75.00	43376.0
76.00	3557.0
76.90	461.0
78.00	302.0
78.90	3675.0
79.90	873.0
80.90	3721.0
81.90	733.0
82.80	124.0
86.10	127.0
87.00	2814.0
87.90	2667.0
90.80	355.0
92.00	2755.0
93.00	3656.0
94.00	10189.0
95.00	75736.0
96.00	5300.0
97.00	148.0
103.80	446.0
104.80	140.0
105.80	417.0
109.70	132.0
110.80	145.0
112.70	117.0
114.70	129.0
115.80	344.0
116.80	632.0
117.80	331.0
118.80	478.0
127.80	311.0
128.80	195.0
129.90	326.0
130.90	120.0
134.80	187.0
136.70	176.0
140.90	1041.0
141.70	182.0
142.80	1058.0
144.90	130.0
145.90	134.0
147.80	193.0
154.70	179.0
156.90	153.0
158.80	120.0
160.80	112.0
171.80	305.0
173.90	65848.0
174.90	5258.0
175.90	64096.0
176.90	3951.0

Instrument :
MSVOA_U
ClientSampleId :
BFB302

m/z	Abundance
36.00	703.0
37.00	4760.0
38.00	4177.0
39.00	1769.0
39.90	250.0
44.00	832.0
45.00	840.0
46.90	900.0
47.90	486.0
49.00	3373.0
50.00	16856.0
51.00	4879.0
52.00	194.0
54.90	194.0
55.90	1365.0
57.00	2357.0
59.90	815.0
61.00	4015.0
62.00	4236.0
63.00	2811.0
64.00	230.0
65.00	158.0
67.00	278.0
68.00	8160.0
69.00	8157.0
69.90	658.0
72.00	477.0
73.00	3699.0
74.00	14551.0
75.00	41432.0
76.00	3352.0
76.90	455.0
77.90	277.0
78.90	3442.0
79.90	886.0
80.90	3562.0
81.90	746.0
82.80	113.0
86.10	152.0
87.00	2783.0
87.90	2610.0
90.80	386.0
92.00	2551.0
93.00	3519.0
94.00	9925.0
95.00	72448.0
96.00	4967.0
97.00	123.0
103.90	435.0
104.80	122.0
105.80	375.0
109.70	143.0
110.80	132.0
114.80	128.0
115.70	319.0
116.80	554.0
117.80	298.0
118.80	428.0
127.80	309.0
128.80	210.0
129.90	306.0
130.90	114.0
134.80	191.0
136.70	161.0
140.90	962.0
141.70	160.0
142.90	1011.0
145.00	132.0
145.90	114.0
147.80	198.0
154.80	166.0
156.90	121.0
158.80	165.0
171.20	158.0
171.80	316.0
173.90	64416.0
174.90	4929.0
175.90	63296.0
176.90	4148.0
177.90	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB302

m/z	Abundance
43.90	198.0

Instrument :
MSVOA_U
ClientSampleId :
BFB302