


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022719\
 Data File : VU029678.D
 Acq On : 26 Feb 2019 13:33
 Operator : JC/SP
 Sample : BFB50
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM021519WMA.M
 Title : VOC Analysis
 Last Update : Thu Feb 28 00:50:18 2019

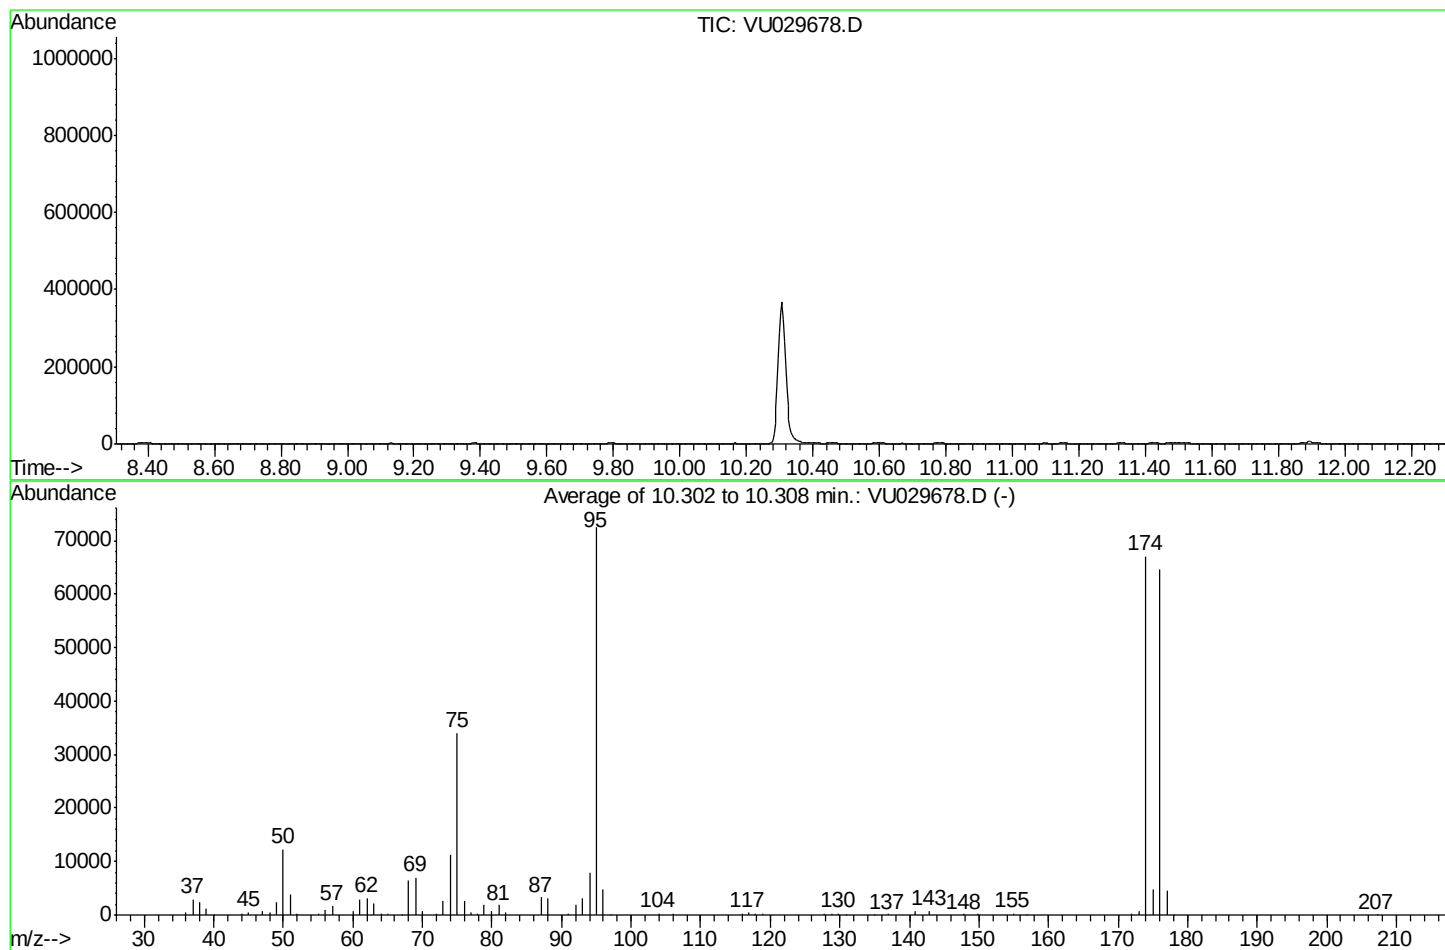

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	12283	PASS
75	95	30	80	47.0	34080	PASS
95	95	100	100	100.0	72477	PASS
96	95	5	9	6.7	4872	PASS
173	174	0.00	2	0.9	611	PASS
174	95	50	120	92.6	67096	PASS
175	174	5	9	7.1	4761	PASS
176	174	95	101	96.3	64613	PASS
177	176	5	9	7.1	4564	PASS

m/z	Abundance
36.00	435.0
37.00	2949.0
38.00	2448.0
39.00	1163.0
39.90	238.0
43.90	910.0
45.00	548.0
47.10	797.0
48.10	400.0
49.00	2394.0
50.00	12250.0
51.00	3883.0
52.00	105.0
55.00	171.0
56.00	959.0
57.00	1610.0
60.00	611.0
61.00	2761.0
62.00	2935.0
63.00	2077.0
64.00	158.0
65.00	262.0
66.90	108.0
68.00	6203.0
69.00	6901.0
70.00	690.0
72.00	300.0
73.00	2527.0
74.00	10858.0
75.00	33528.0
76.00	2867.0
77.10	394.0
77.90	264.0
78.90	1886.0
79.90	645.0
81.00	1881.0
81.90	456.0
87.00	3306.0
88.00	3113.0
91.10	253.0
92.00	1940.0
93.00	2917.0
94.00	7519.0
95.00	69704.0
96.00	4625.0
97.10	127.0
104.00	283.0
106.00	238.0
115.90	244.0
116.90	415.0
117.80	238.0
119.00	211.0
127.80	207.0
129.00	141.0
129.90	249.0
136.90	246.0
140.90	652.0
142.90	679.0
147.80	123.0
149.80	132.0
155.00	248.0
171.80	298.0
172.90	587.0
174.00	63200.0
175.00	4698.0
176.00	61176.0
177.00	4483.0
206.90	118.0

Instrument :
MSVOA_U
ClientSampleId :

m/z	Abundance
36.00	413.0
37.00	3016.0
38.00	2590.0
39.00	1148.0
39.90	208.0
43.90	883.0
45.00	620.0
47.10	767.0
48.00	425.0
49.00	2604.0
50.00	12647.0
51.00	3830.0
51.90	157.0
55.00	164.0
56.00	1049.0
57.00	1790.0
60.00	654.0
61.00	3096.0
62.00	3274.0
63.00	2258.0
64.00	174.0
65.00	315.0
66.90	114.0
68.00	6548.0
69.00	7251.0
70.00	702.0
71.90	336.0
73.00	2726.0
74.00	11623.0
75.00	35120.0
76.00	2803.0
77.10	444.0
77.90	275.0
78.90	1848.0
79.90	710.0
81.00	1959.0
81.90	450.0
87.00	3470.0
88.00	3319.0
91.00	271.0
92.00	2035.0
93.00	3247.0
94.00	8083.0
95.00	74768.0
96.00	4977.0
97.10	123.0
104.00	313.0
106.00	230.0
115.90	284.0
116.90	439.0
117.80	271.0
119.00	219.0
127.80	219.0
128.90	125.0
129.90	254.0
130.80	127.0
134.90	120.0
136.90	232.0
140.90	681.0
142.90	791.0
147.80	142.0
149.80	142.0
154.90	251.0
171.90	326.0
173.00	644.0
174.00	69216.0
175.00	4866.0
176.00	66496.0
177.00	4768.0
178.00	138.0
207.20	142.0

Instrument :
MSVOA_U
ClientSampleId :

m/z	Abundance
36.00	429.0
37.00	2864.0
38.00	2500.0
38.90	1059.0
40.00	204.0
44.00	834.0
45.00	591.0
47.00	683.0
47.90	432.0
49.00	2521.0
50.00	11952.0
51.00	3528.0
51.90	195.0
55.00	113.0
56.00	1058.0
57.10	1804.0
60.00	650.0
61.00	3062.0
62.00	3193.0
63.00	2281.0
64.00	191.0
65.00	301.0
67.00	113.0
68.00	6382.0
69.00	6974.0
70.00	598.0
71.90	323.0
73.00	2723.0
74.00	11254.0
75.00	33592.0
76.00	2609.0
77.00	440.0
78.00	241.0
78.90	1740.0
79.90	672.0
81.00	1839.0
81.90	412.0
87.00	3197.0
87.90	3087.0
90.90	314.0
92.00	1828.0
93.00	3237.0
94.00	8215.0
95.00	72960.0
96.00	5015.0
104.00	318.0
106.00	222.0
116.00	302.0
116.80	421.0
117.80	272.0
118.90	275.0
127.90	240.0
128.90	120.0
129.80	269.0
130.80	137.0
134.90	144.0
136.90	159.0
140.90	692.0
142.90	734.0
147.90	160.0
149.80	130.0
154.90	239.0
156.90	109.0
171.90	306.0
173.00	603.0
174.00	68872.0
175.00	4721.0
176.00	66168.0
177.00	4443.0
178.00	159.0
207.20	155.0

Instrument :
MSVOA_U
ClientSampleId :

Scan 2854 (10.266 min): VU029678.D
BFB50

m/z	Abundance
39.90	164.0
44.00	632.0
207.00	199.0

Instrument :
MSVOA_U
ClientSampleId :