


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022719\
Data File : VU029700.D
Acq On : 27 Feb 2019 10:47
Operator : JC/SP
Sample : BFB51
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022519W.M
Title : SW846 8260
Last Update : Thu Feb 28 04:05:45 2019

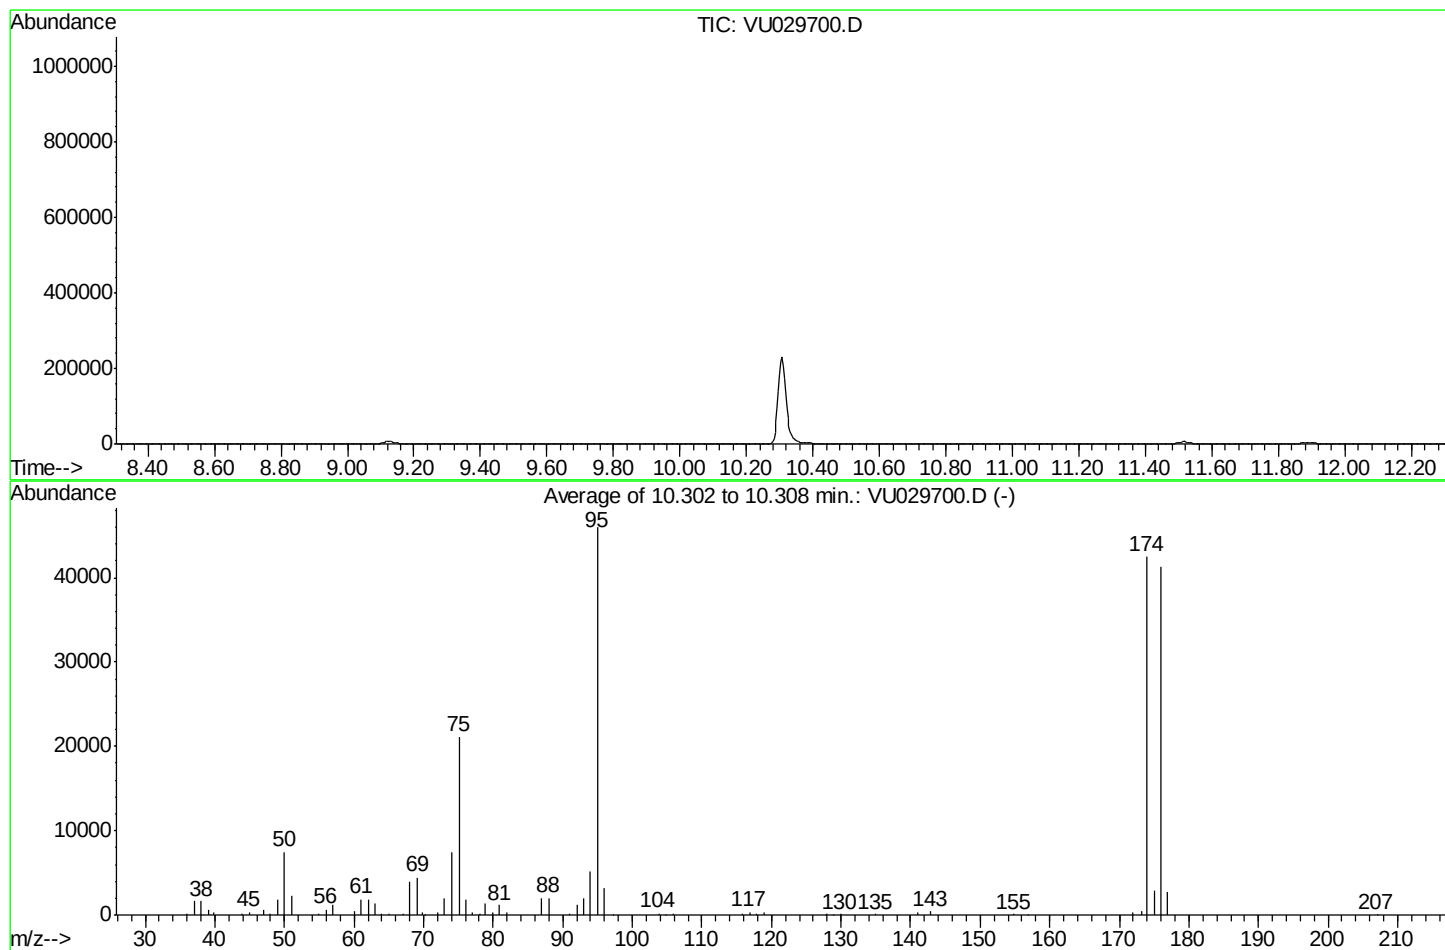

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	7480	PASS
75	95	30	60	46.0	21133	PASS
95	95	100	100	100.0	45973	PASS
96	95	5	9	6.8	3138	PASS
173	174	0.00	2	1.1	449	PASS
174	95	50	100	92.4	42464	PASS
175	174	5	9	6.8	2906	PASS
176	174	95	101	97.1	41242	PASS
177	176	5	9	6.5	2695	PASS

m/z	Abundance
35.90	214.0
37.00	1492.0
38.00	1513.0
39.00	625.0
39.90	237.0
44.00	653.0
44.90	364.0
47.00	568.0
47.90	188.0
49.00	1868.0
50.00	7208.0
51.00	2238.0
55.10	111.0
56.00	583.0
57.00	1238.0
60.00	414.0
61.10	1715.0
62.00	1792.0
63.00	1316.0
64.00	164.0
64.90	160.0
68.00	3826.0
69.10	4178.0
69.90	327.0
72.00	198.0
73.00	1885.0
74.00	7085.0
75.10	20816.0
76.10	1773.0
77.00	257.0
78.20	179.0
78.90	1223.0
79.90	364.0
80.90	1136.0
81.90	297.0
87.00	1835.0
87.90	1850.0
90.90	208.0
92.00	1189.0
93.00	1952.0
94.00	4853.0
95.00	44824.0
96.00	3008.0
97.20	115.0
103.80	171.0
105.80	163.0
115.90	147.0
116.90	353.0
117.80	166.0
118.90	218.0
127.80	189.0
130.00	117.0
134.90	123.0
140.90	374.0
142.90	361.0
172.00	262.0
173.20	479.0
174.00	39680.0
175.00	2781.0
176.00	39080.0
176.90	2619.0
207.00	195.0

Instrument :
MSVOA_U
ClientSampleId :

m/z	Abundance
35.90	202.0
37.00	1641.0
38.00	1727.0
39.00	672.0
39.90	261.0
44.00	635.0
44.90	367.0
47.10	564.0
48.00	244.0
49.00	1795.0
50.00	7711.0
51.00	2237.0
55.00	129.0
56.00	683.0
57.00	1223.0
60.00	476.0
61.10	1931.0
62.00	1879.0
63.10	1371.0
63.90	192.0
65.00	157.0
67.10	119.0
68.00	4136.0
69.10	4614.0
69.90	232.0
72.10	269.0
73.00	2008.0
74.00	7651.0
75.10	21752.0
76.10	1912.0
77.00	292.0
78.10	185.0
78.90	1392.0
79.90	334.0
80.90	1224.0
81.90	306.0
87.00	1954.0
88.00	2143.0
90.90	183.0
92.00	1227.0
93.00	2006.0
94.00	5410.0
95.00	47376.0
96.00	3256.0
97.20	120.0
103.80	188.0
104.80	107.0
105.90	181.0
115.90	151.0
116.90	351.0
117.80	155.0
118.90	276.0
128.00	166.0
130.00	130.0
135.00	124.0
140.90	370.0
142.90	454.0
154.90	134.0
156.90	103.0
172.00	316.0
173.20	448.0
174.00	43552.0
175.00	2955.0
176.00	42312.0
177.00	2716.0
207.00	157.0

Instrument :
MSVOA_U
ClientSampleId :

m/z	Abundance
35.90	203.0
37.00	1722.0
38.00	1731.0
39.00	608.0
39.90	211.0
44.00	536.0
45.00	332.0
47.10	504.0
48.00	257.0
49.00	1631.0
50.00	7523.0
51.00	2150.0
54.90	125.0
56.00	739.0
57.00	1093.0
60.00	416.0
61.00	1950.0
62.00	1820.0
63.10	1401.0
63.90	211.0
65.10	143.0
67.10	147.0
68.00	4052.0
69.10	4626.0
69.90	159.0
70.20	159.0
72.10	308.0
73.00	1879.0
74.00	7481.0
75.10	20832.0
76.10	1878.0
77.10	283.0
78.00	165.0
78.90	1321.0
79.90	281.0
80.90	1282.0
81.90	262.0
86.90	2061.0
88.00	2168.0
90.90	186.0
92.00	1173.0
93.00	1900.0
94.00	5385.0
95.00	45720.0
96.00	3150.0
103.80	159.0
104.90	131.0
105.90	174.0
115.90	161.0
116.90	288.0
117.90	140.0
118.90	283.0
128.00	139.0
128.90	106.0
129.90	114.0
141.00	369.0
142.90	492.0
154.90	157.0
156.80	126.0
172.00	333.0
173.10	421.0
174.00	44160.0
175.00	2982.0
176.00	42336.0
177.00	2752.0
207.10	100.0

Instrument :
MSVOA_U
ClientSampleId :

m/z	Abundance
43.90	497.0
207.00	142.0

Instrument :
MSVOA_U
ClientSampleId :