

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU022720\
 Data File : VU036938.D
 Acq On : 27 Feb 2020 13:09
 Operator : JC/MD
 Sample : L1686-04 20X
 Misc : 9.49g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GAW03

Quant Time: Feb 27 22:37:01 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Feb 27 22:00:13 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	260709	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	249787	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	95055	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	80365	36.71	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	73.42%
7) Chloroethane-d5	1.93	69	76110	42.01	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	84.02%
11) 1,1-Dichloroethene-d2	2.59	63	108559	29.61	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	59.22%#
21) 2-Butanone-d5	4.67	46	143102	97.44	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.44%
24) Chloroform-d	5.11	84	143689	42.98	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.96%
26) 1,2-Dichloroethane-d4	5.74	65	103903	45.92	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.84%
32) Benzene-d6	5.76	84	321125	44.46	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.92%
36) 1,2-Dichloropropane-d6	6.72	67	107224	45.82	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.64%
41) Toluene-d8	7.92	98	288955	43.12	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.24%
43) trans-1,3-Dichloropropene-	8.20	79	45781	42.10	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.20%
47) 2-Hexanone-d5	8.66	63	106976	93.49	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.49%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	152362	46.18	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.36%
64) 1,2-Dichlorobenzene-d4	12.21	152	88678	47.72	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.44%


Target Compounds					Ovalue
34) Trichloroethene	6.57	95	12043	6.209 ug/L	97
46) Tetrachloroethene	8.57	164	240737	188.416 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU022720\
Data File : VU036938.D
Acq On : 27 Feb 2020 13:09
Operator : JC/MD
Sample : L1686-04 20X
Misc : 9.49g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GAW03

Quant Time: Feb 27 22:37:01 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Feb 27 22:00:13 2020
Response via : Initial Calibration

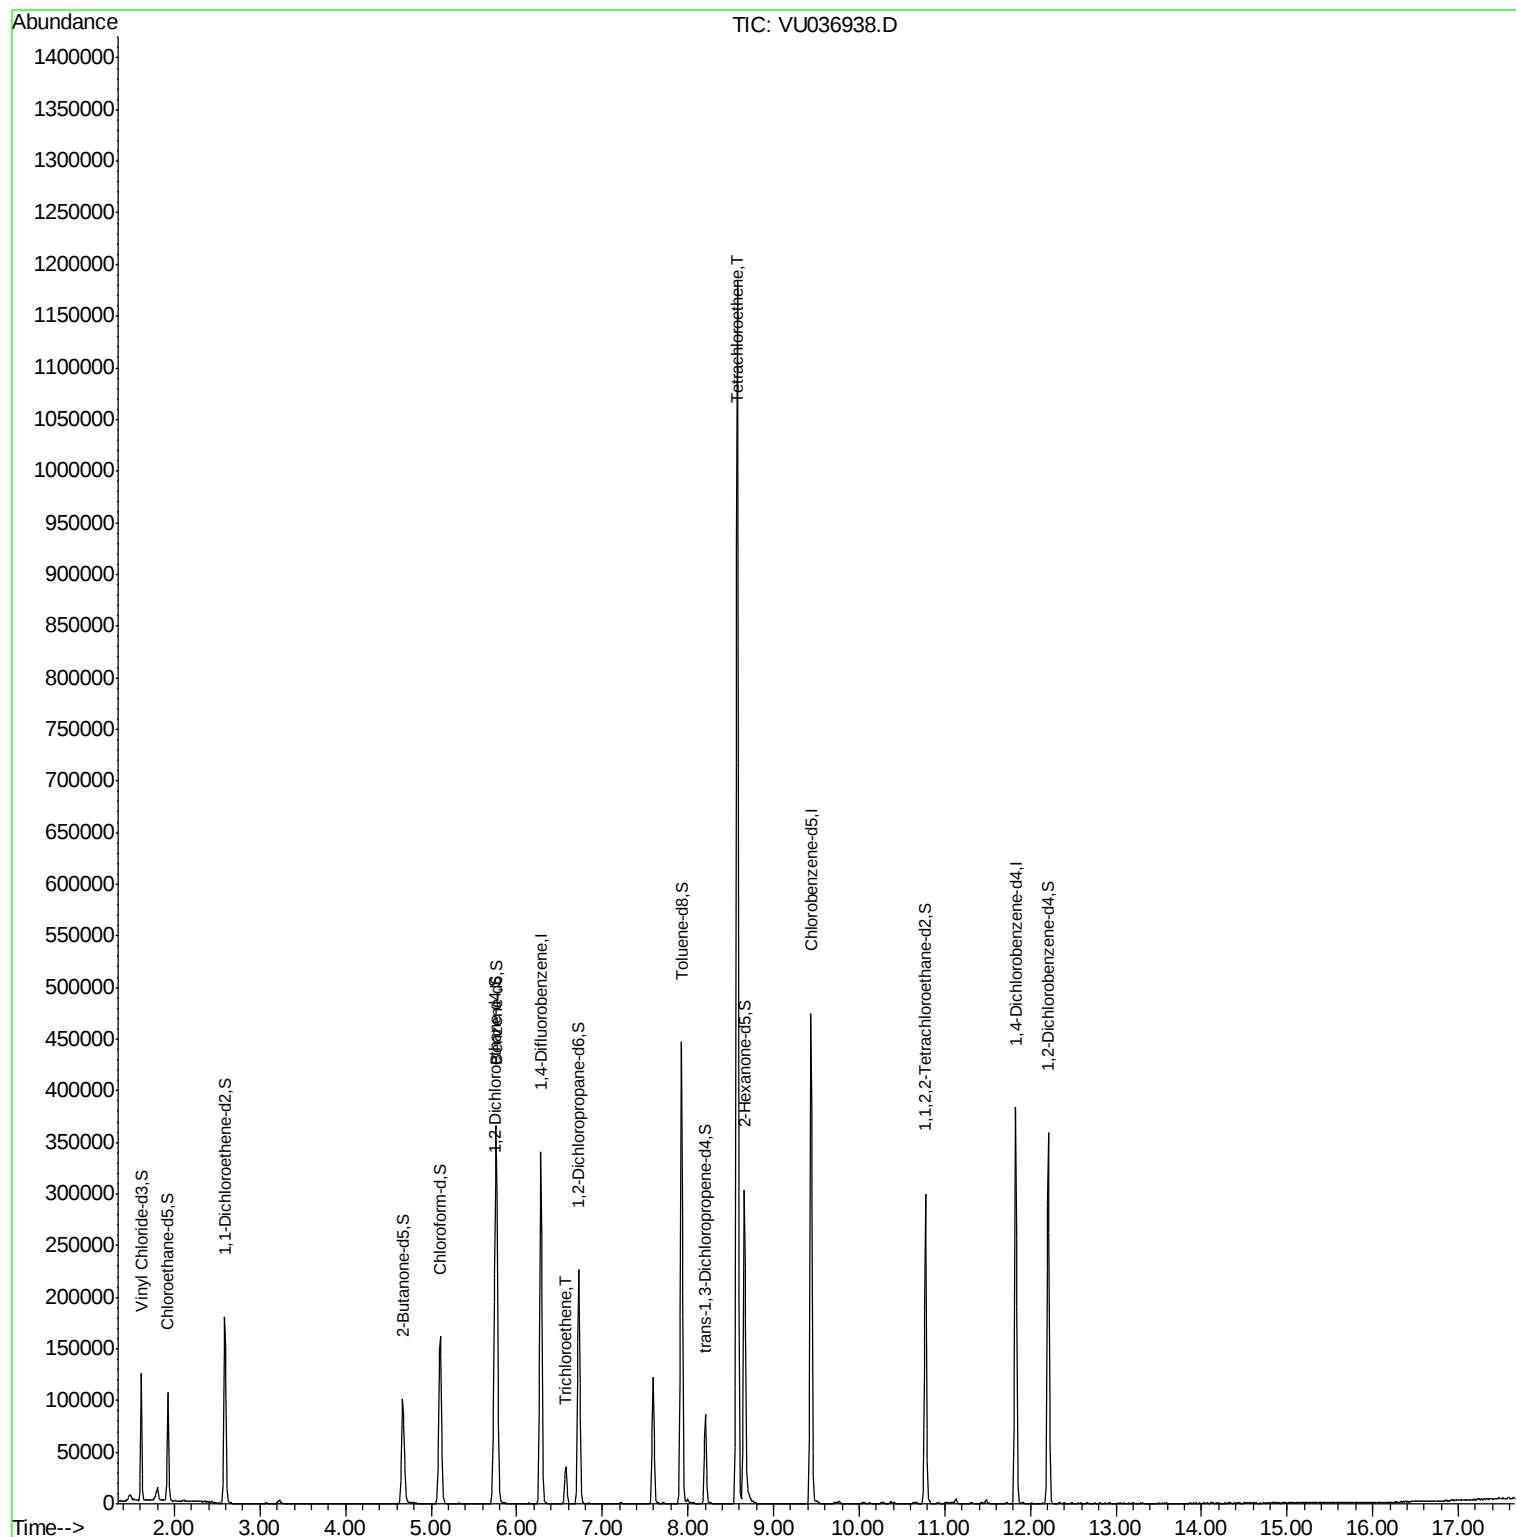

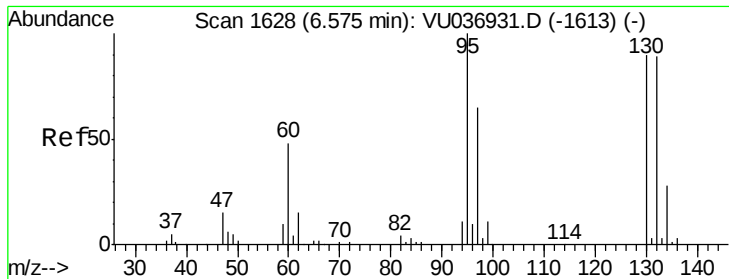

#34

Trichloroethene

Concen: 6.209 ug/L

RT: 6.57 min Scan# 1628

Delta R.T. -0.00 min

Lab File: VU036938.D

Acq: 27 Feb 2020 13:09

Instrument :

MSVOA_U

ClientSampled :

GAW03

Tot Ion: 95 Resp: 12043


Ion Ratio Lower Upper

95 100

97 66.5 44.1 81.9

132 89.5 60.6 112.6

130 94.4 64.9 120.5



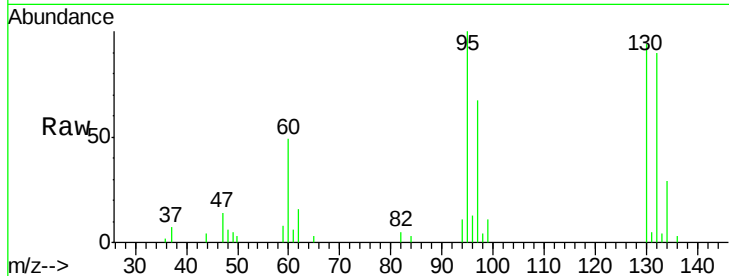


Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 97.00 (96.70 to 97.70): VU0

Ion 132.00 (131.70 to 132.70): V

Ion 130.00 (129.70 to 130.70): V

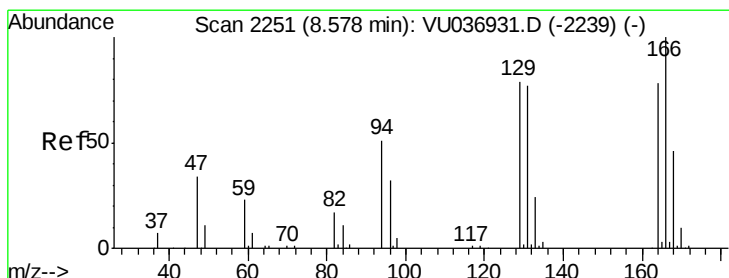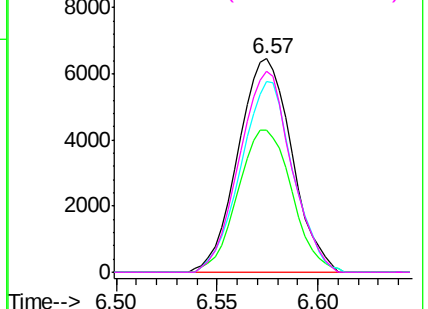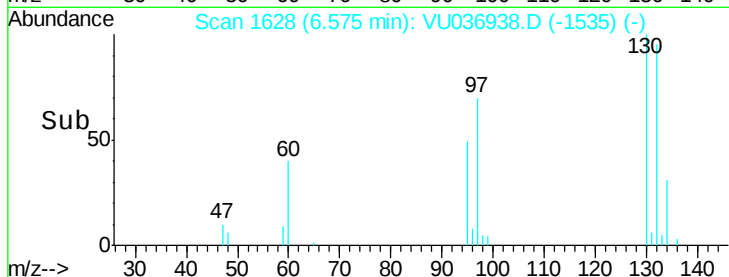

#46

Tetrachloroethene

Concen: 188.416 ug/L

RT: 8.57 min Scan# 2250

Delta R.T. -0.00 min

Lab File: VU036938.D

Acq: 27 Feb 2020 13:09

Tgt Ion: 164 Resp: 240737


Ion Ratio Lower Upper

164 100

129 103.8 72.0 133.8

131 100.6 67.9 126.1

166 125.6 87.1 161.7

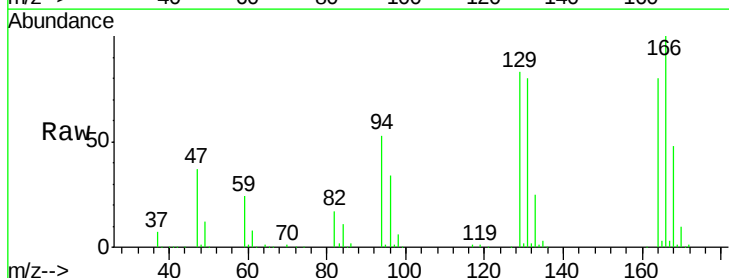

Abundance Ion 164.00 (163.70 to 164.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 131.00 (130.70 to 131.70): V

Ion 166.00 (165.70 to 166.70): V

