


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU022720\
 Data File : VU036930.D
 Acq On : 27 Feb 2020 09:18
 Operator : JC/MD
 Sample : BFB53
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB53

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
 Title : VOC Analysis
 Last Update : Mon Mar 02 16:10:39 2020

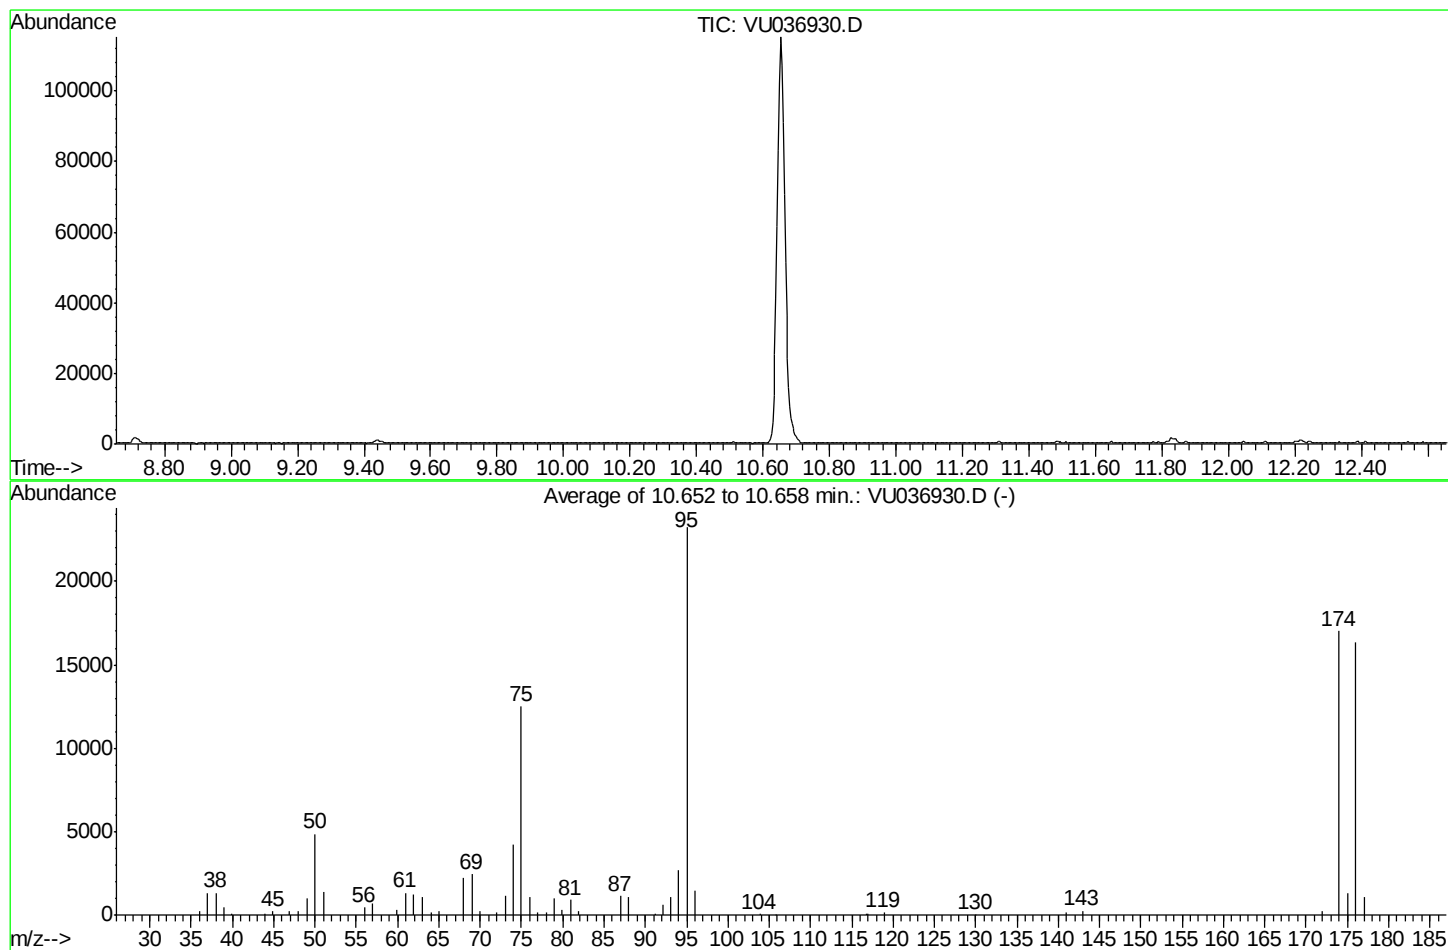

AutoFind: Scans 2896, 2897, 2898; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	4845	PASS
75	95	30	80	53.7	12479	PASS
95	95	100	100	100.0	23240	PASS
96	95	5	9	6.4	1492	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.3	17034	PASS
175	174	5	9	7.5	1273	PASS
176	174	95	101	95.8	16320	PASS
177	176	5	9	6.5	1059	PASS

m/z	Abundance
36.00	281.0
37.00	1340.0
38.00	1297.0
39.00	480.0
44.00	427.0
44.90	224.0
46.90	259.0
48.00	215.0
49.00	1109.0
50.00	5108.0
51.00	1455.0
55.90	409.0
57.00	688.0
60.00	270.0
60.90	1416.0
62.00	1290.0
63.00	1062.0
64.00	153.0
64.90	245.0
68.00	2158.0
69.00	2534.0
70.00	200.0
71.90	161.0
73.00	1193.0
74.10	4372.0
75.00	12873.0
76.00	1104.0
77.00	179.0
77.90	126.0
78.90	902.0
79.90	316.0
80.90	963.0
82.00	217.0
87.00	989.0
88.00	1125.0
91.20	139.0
92.10	646.0
93.00	1090.0
94.00	2762.0
95.00	23760.0
96.00	1619.0
103.90	130.0
116.80	136.0
118.90	140.0
130.00	106.0
141.00	188.0
142.90	257.0
172.00	208.0
174.00	16712.0
175.00	1205.0
176.00	16138.0
177.00	1097.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53

m/z	Abundance
36.00	278.0
37.00	1327.0
38.00	1376.0
39.00	470.0
39.90	105.0
43.90	451.0
44.90	224.0
46.90	261.0
48.00	217.0
49.00	1013.0
50.00	4982.0
51.00	1453.0
56.00	468.0
57.00	751.0
60.00	269.0
61.00	1390.0
62.00	1274.0
63.00	1135.0
64.00	160.0
65.00	214.0
68.00	2327.0
69.00	2510.0
70.00	211.0
72.00	172.0
73.00	1189.0
74.00	4402.0
75.00	12856.0
76.00	1085.0
77.00	188.0
77.90	139.0
78.90	993.0
79.90	329.0
80.90	941.0
82.00	206.0
87.00	1151.0
88.00	1102.0
91.20	114.0
92.10	598.0
93.00	1080.0
94.10	2758.0
95.00	23808.0
96.00	1506.0
105.80	105.0
117.00	130.0
118.90	129.0
141.00	163.0
142.90	257.0
171.90	204.0
174.00	17536.0
175.00	1297.0
176.00	16904.0
177.00	1084.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53

m/z	Abundance
35.00	236.0
37.00	1187.0
38.00	1280.0
39.00	427.0
39.00	113.0
43.00	436.0
44.00	223.0
46.00	249.0
48.00	179.0
49.00	912.0
50.00	4445.0
51.00	1294.0
56.00	462.0
57.00	726.0
59.00	275.0
61.00	1214.0
61.00	1157.0
63.00	1077.0
64.00	158.0
64.00	166.0
68.00	2275.0
69.00	2301.0
70.00	197.0
72.00	153.0
73.00	1109.0
74.00	4011.0
75.00	11709.0
76.00	939.0
77.00	157.0
78.00	152.0
78.00	1009.0
79.00	292.0
80.00	858.0
81.00	181.0
87.00	1240.0
88.00	961.0
92.10	542.0
93.00	1016.0
94.10	2510.0
95.00	22152.0
96.00	1351.0
117.00	135.0
119.00	131.0
141.00	147.0
142.90	222.0
171.90	206.0
174.00	16856.0
175.00	1318.0
176.00	15918.0
177.00	996.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53

m/z	Abundance
44.00	377.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53