
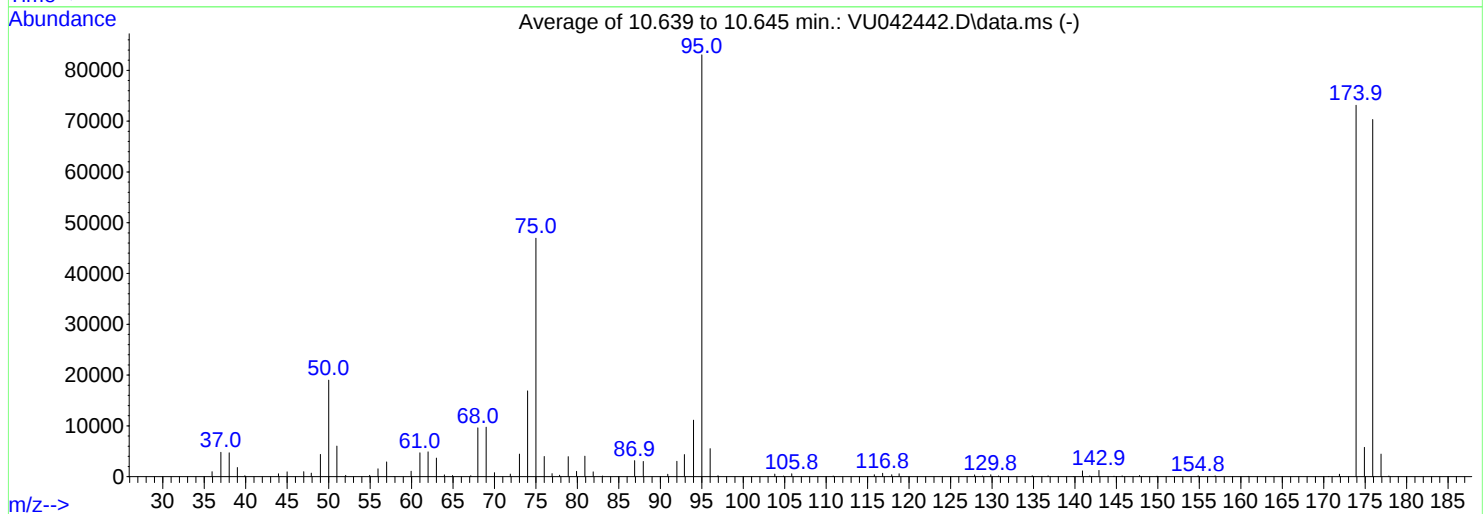


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022721\
 Data File : VU042442.D
 Acq On : 26 Feb 2021 11:22
 Operator : SY/MD
 Sample : BFB39
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB391

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022621WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Feb 27 00:17:17 2021

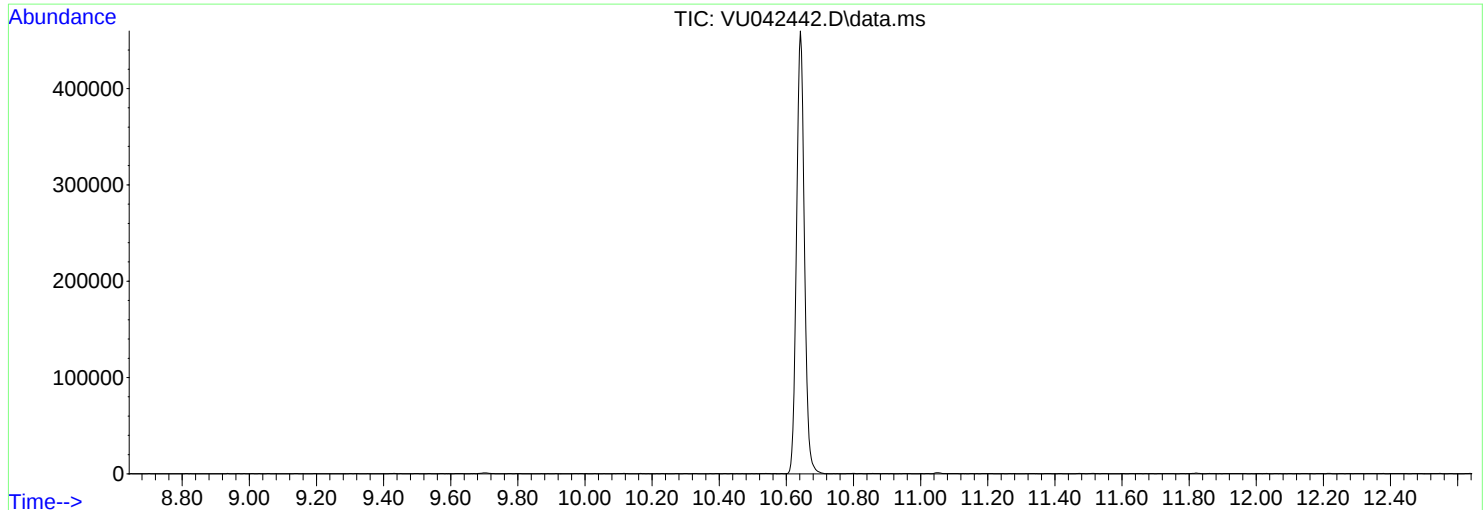

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	18984	PASS
75	95	30	80	56.5	46957	PASS
95	95	100	100	100.0	83056	PASS
96	95	5	9	6.7	5528	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	88.0	73117	PASS
175	174	5	9	7.9	5756	PASS
176	174	95	101	96.2	70325	PASS
177	176	5	9	6.3	4454	PASS

m/z	Abundance
35.90	987.0
37.00	4865.0
38.00	4810.0
39.00	1861.0
39.90	192.0
44.00	726.0
45.00	887.0
47.00	893.0
47.90	636.0
49.00	4240.0
50.00	19240.0
51.00	5953.0
52.00	239.0
54.90	288.0
56.00	1525.0
57.00	2983.0
57.90	109.0
59.90	997.0
61.00	4654.0
62.00	4707.0
63.00	3595.0
63.90	365.0
65.00	208.0
67.10	263.0
68.00	9497.0
69.00	9541.0
70.00	886.0
71.90	510.0
73.00	4609.0
74.00	17136.0
75.00	47152.0
76.00	4112.0
76.90	533.0
77.80	282.0
78.90	4041.0
79.90	972.0
80.90	4113.0
81.90	913.0
83.10	103.0
86.90	3048.0
87.90	2954.0
90.90	453.0
92.00	2982.0
92.90	4388.0
94.00	11182.0
95.00	81752.0
96.00	5679.0
97.00	189.0
103.80	513.0
104.80	120.0
105.90	598.0
110.80	114.0
115.80	391.0
116.80	653.0
117.90	400.0
118.80	577.0
127.90	381.0
128.90	128.0
129.90	352.0
130.80	147.0
134.90	195.0
136.80	189.0
140.90	1114.0
141.80	156.0
142.90	1125.0
145.70	127.0
147.80	230.0
149.90	142.0
154.90	177.0
156.90	164.0
159.00	121.0
160.90	133.0
171.90	454.0
173.90	70200.0
174.90	5612.0
175.90	68200.0
176.90	4355.0
177.80	149.0

Instrument :
MSVOA_U
ClientSampleId :
BFB391

m/z	Abundance
35.90	979.0
37.00	4906.0
38.00	4792.0
39.00	1829.0
39.90	200.0
44.00	806.0
45.00	973.0
47.00	1036.0
47.90	692.0
49.00	4474.0
50.00	19528.0
51.00	6244.0
52.10	276.0
54.90	272.0
55.90	1575.0
57.00	2967.0
60.00	1120.0
61.00	4863.0
62.00	5017.0
63.00	3759.0
64.00	345.0
64.90	209.0
67.20	287.0
68.00	9901.0
69.00	10090.0
70.00	816.0
71.90	525.0
73.00	4591.0
74.00	17408.0
75.00	48624.0
76.00	4134.0
77.00	618.0
77.80	301.0
78.90	4048.0
79.90	1091.0
80.90	4155.0
81.90	974.0
83.00	133.0
86.90	3269.0
88.00	3054.0
90.90	482.0
92.00	3148.0
92.90	4510.0
94.00	11484.0
95.00	85936.0
96.00	5651.0
96.90	188.0
103.80	527.0
104.90	127.0
105.90	586.0
110.90	139.0
115.80	384.0
116.80	689.0
117.90	390.0
118.80	610.0
127.90	376.0
128.80	137.0
129.90	383.0
130.80	150.0
134.90	201.0
136.70	159.0
139.80	112.0
140.90	1165.0
141.80	170.0
142.90	1273.0
144.70	118.0
145.70	168.0
147.80	247.0
149.90	133.0
152.80	100.0
154.80	207.0
156.90	185.0
160.90	105.0
171.90	493.0
173.90	75144.0
174.90	5898.0
175.90	72320.0
176.90	4588.0
177.90	136.0

Instrument :
MSVOA_U
ClientSampleId :
BFB391

m/z	Abundance
36.00	938.0
37.00	4612.0
38.00	4458.0
39.00	1750.0
39.90	145.0
44.00	834.0
45.00	981.0
47.00	975.0
47.90	725.0
49.00	4481.0
50.00	18184.0
51.00	5886.0
52.10	286.0
55.00	235.0
55.90	1517.0
57.00	2766.0
60.00	1080.0
61.00	4582.0
62.00	4950.0
63.00	3615.0
64.00	323.0
64.90	215.0
68.00	9441.0
69.00	9555.0
70.00	699.0
71.90	451.0
73.00	4107.0
74.00	16084.0
75.00	45096.0
76.00	3703.0
77.00	602.0
77.90	279.0
78.90	3721.0
79.90	1062.0
80.90	3844.0
81.90	921.0
83.00	134.0
86.90	3127.0
88.00	2966.0
90.90	478.0
92.00	2925.0
92.90	4132.0
94.00	10743.0
95.00	81480.0
96.00	5254.0
97.00	166.0
103.80	480.0
104.90	123.0
105.80	499.0
110.90	142.0
115.80	333.0
116.80	621.0
117.90	379.0
118.80	524.0
127.90	321.0
128.80	159.0
129.80	368.0
130.80	154.0
134.80	185.0
136.80	125.0
140.90	1101.0
141.80	182.0
142.90	1317.0
144.70	131.0
145.70	188.0
147.80	232.0
154.80	194.0
156.90	173.0
170.60	120.0
171.90	448.0
173.90	74008.0
174.90	5758.0
175.90	70456.0
176.90	4418.0
177.90	107.0

Instrument :
MSVOA_U
ClientSampleId :
BFB391

m/z	Abundance
43.90	215.0

Instrument :
MSVOA_U
ClientSampleId :
BFB391