
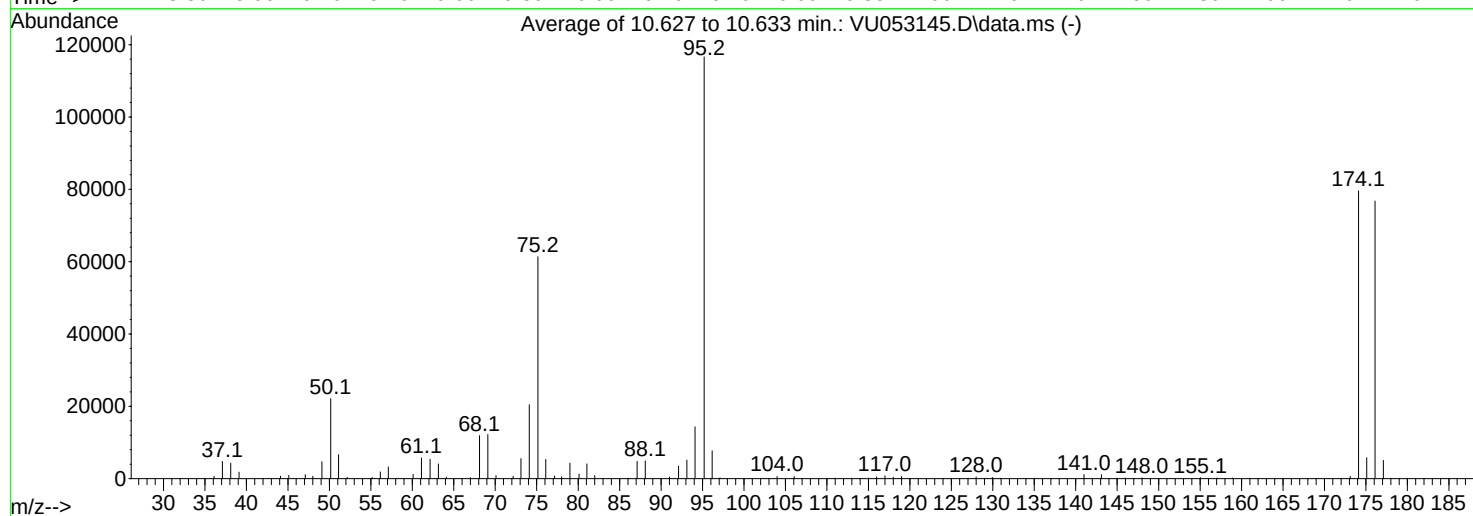


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022723\
 Data File : VU053145.D
 Acq On : 27 Feb 2023 08:57
 Operator : JC/MD
 Sample : BFB
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U022723DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Tue Feb 28 03:35:42 2023

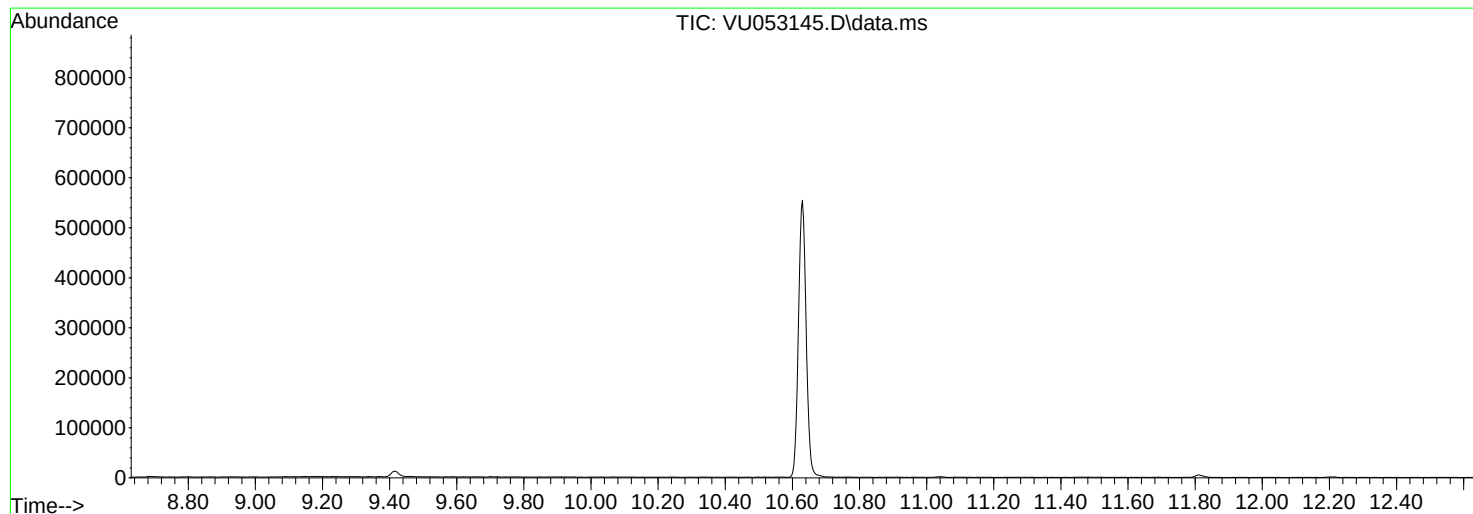

AutoFind: Scans 2966, 2967, 2968; Background Corrected with Scan 2952

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	22120	PASS
75	95	30	60	52.6	61357	PASS
95	95	100	100	100.0	116635	PASS
96	95	5	9	6.6	7706	PASS
173	174	0.00	2	0.8	607	PASS
174	95	50	100	68.3	79613	PASS
175	174	5	9	7.3	5786	PASS
176	174	95	101	96.4	76779	PASS
177	176	5	9	6.6	5037	PASS