

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU022819\
 Data File : VU029727.D
 Acq On : 28 Feb 2019 10:56
 Operator : JC/SP
 Sample : K1577-19
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CWK08

Quant Time: Mar 01 00:34:51 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR022119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Mar 01 00:18:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	256024	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	240008	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	122297	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	70106	4.19	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.80%
7) Chloroethane-d5	1.68	69	69079	4.39	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.80%
11) 1,1-Dichloroethene-d2	2.27	63	111512	3.10	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.00%
20) 2-Butanone-d5	4.19	46	203468	53.82	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.64%
24) Chloroform-d	4.65	84	144776	4.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.20%
26) 1,2-Dichloroethane-d4	5.31	65	78069	4.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.20%
32) Benzene-d6	5.34	84	311298	5.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.00%
36) 1,2-Dichloropropane-d6	6.33	67	96633	5.39	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.80%
41) Toluene-d8	7.56	98	281300	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.20%
43) trans-1,3-Dichloropropene-	7.85	79	36761	4.99	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	99.80%
46) 2-Hexanone-d5	8.31	63	198188	54.94	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	109.88%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	81010	5.03	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.60%
64) 1,2-Dichlorobenzene-d4	11.86	152	119874	4.98	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.60%


Target Compounds					Qvalue
13) Acetone	2.33	43	14641	5.391 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU022819\
Data File : VU029727.D
Acq On : 28 Feb 2019 10:56
Operator : JC/SP
Sample : K1577-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CWK08

Quant Time: Mar 01 00:34:51 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR022119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Mar 01 00:18:18 2019
Response via : Initial Calibration

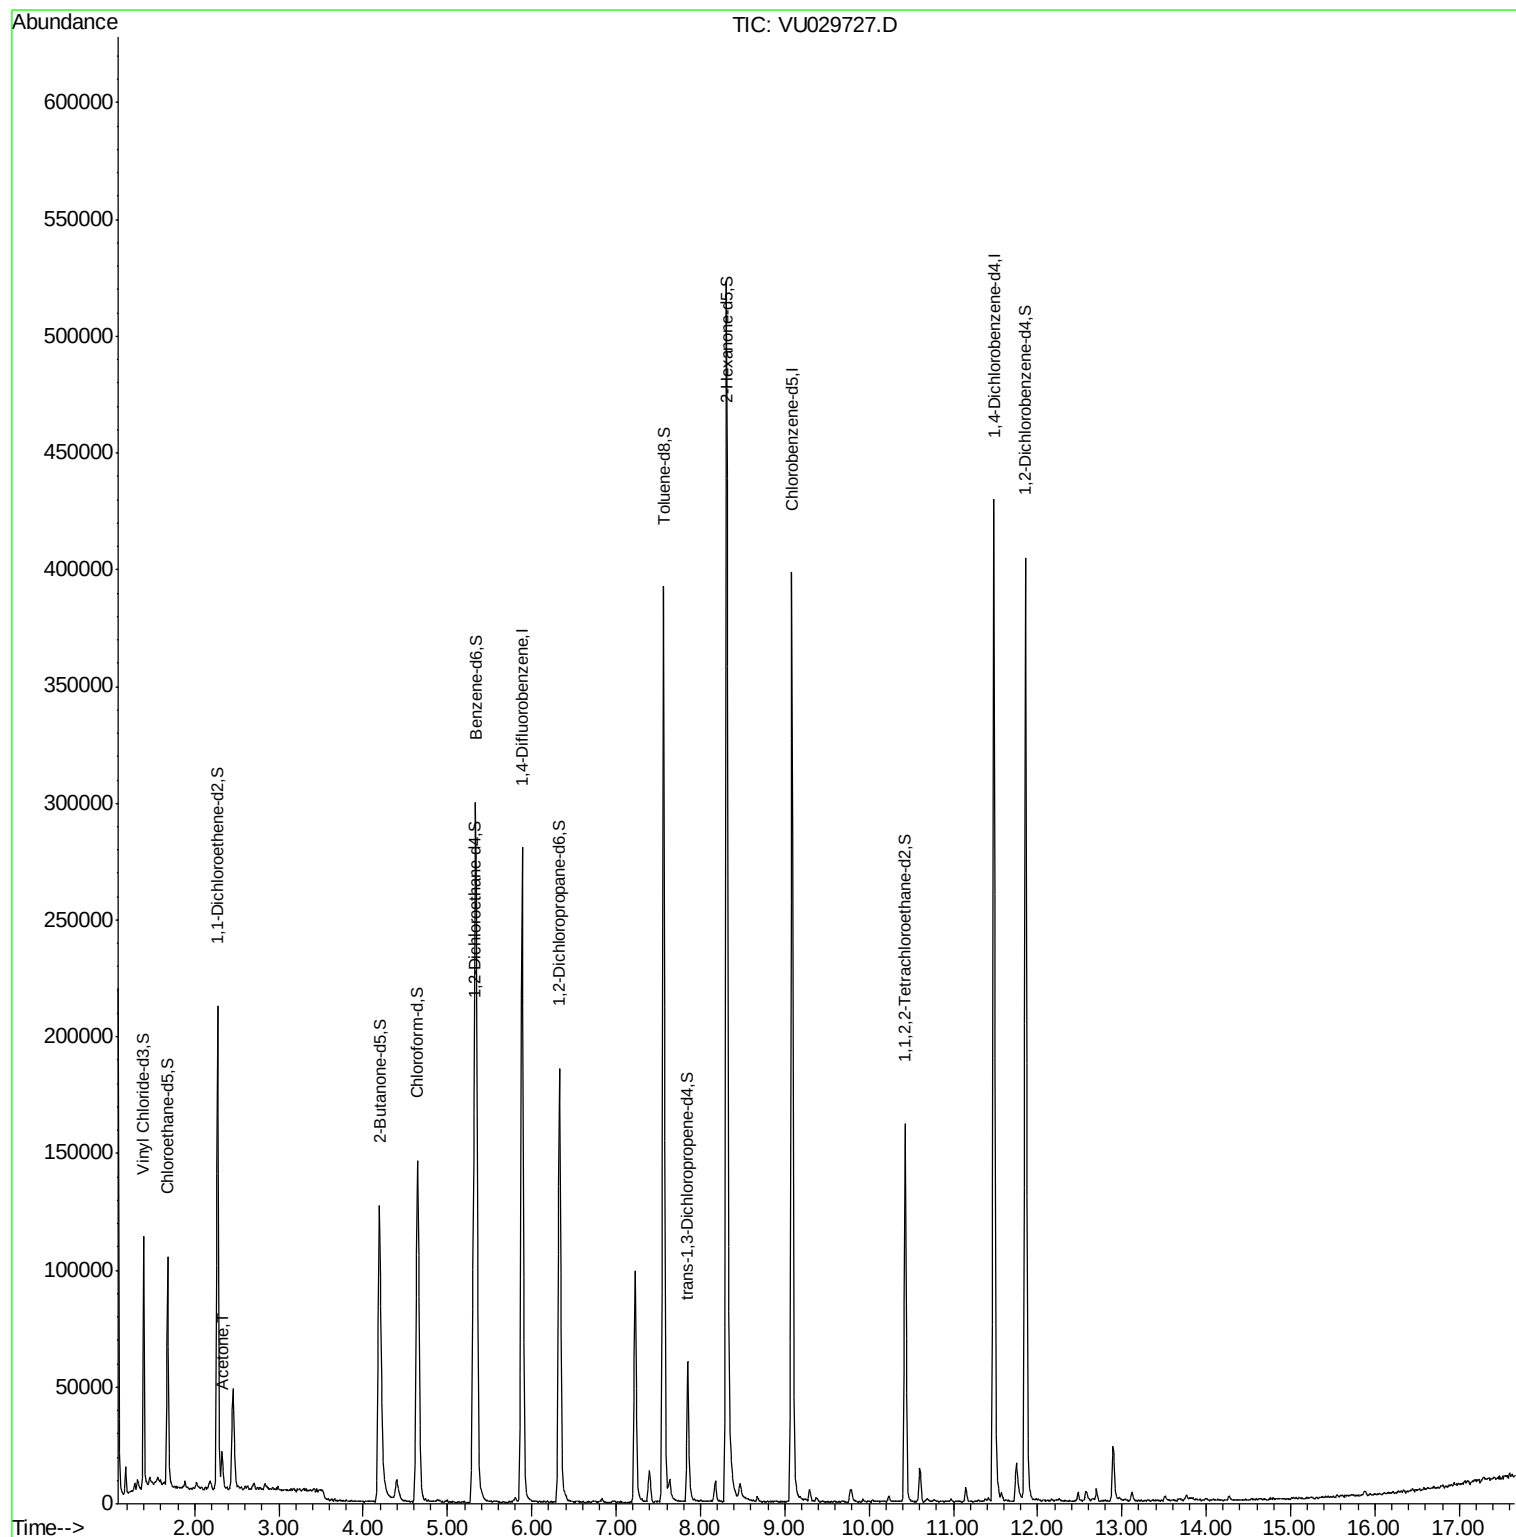

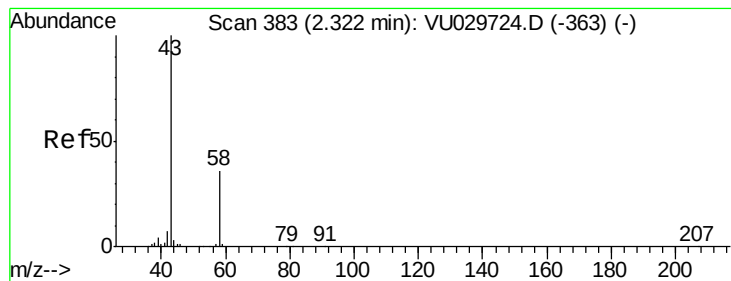

#13
 Acetone
 Concen: 5.391 ug/L
 RT: 2.33 min Scan# 385
 Delta R.T. 0.01 min
 Lab File: VU029727.D
 Acq: 28 Feb 2019 10:56

Instrument :
 MSVOA_U
 ClientSampleId :
 CWK08

Tgt Ion: 43 Resp: 14641
 Ion Ratio Lower Upper
 43 100
 58 36.1 0.0 70.2

