

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU022819\
 Data File : VU029728.D
 Acq On : 28 Feb 2019 11:20
 Operator : JC/SP
 Sample : K1577-20
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CWK11

Quant Time: Mar 01 00:36:56 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR022119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Mar 01 00:18:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	261186	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	252777	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	128388	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	73228	4.29	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.80%
7) Chloroethane-d5	1.68	69	73238	4.56	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.20%
11) 1,1-Dichloroethene-d2	2.27	63	117212	3.20	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.00%
20) 2-Butanone-d5	4.19	46	214275	55.56	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.12%
24) Chloroform-d	4.65	84	150871	5.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.40%
26) 1,2-Dichloroethane-d4	5.31	65	81565	5.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.40%
32) Benzene-d6	5.34	84	332148	5.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.40%
36) 1,2-Dichloropropane-d6	6.33	67	100677	5.33	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.60%
41) Toluene-d8	7.56	98	300488	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.60%
43) trans-1,3-Dichloropropene-	7.85	79	38181	4.92	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	98.40%
46) 2-Hexanone-d5	8.31	63	201857	53.13	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	106.26%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	84224	4.97	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.40%
64) 1,2-Dichlorobenzene-d4	11.86	152	121483	4.81	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.20%


Target Compounds					Qvalue
13) Acetone	2.32	43	13015	4.697 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU022819\
Data File : VU029728.D
Acq On : 28 Feb 2019 11:20
Operator : JC/SP
Sample : K1577-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CWK11

Quant Time: Mar 01 00:36:56 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR022119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Mar 01 00:18:18 2019
Response via : Initial Calibration

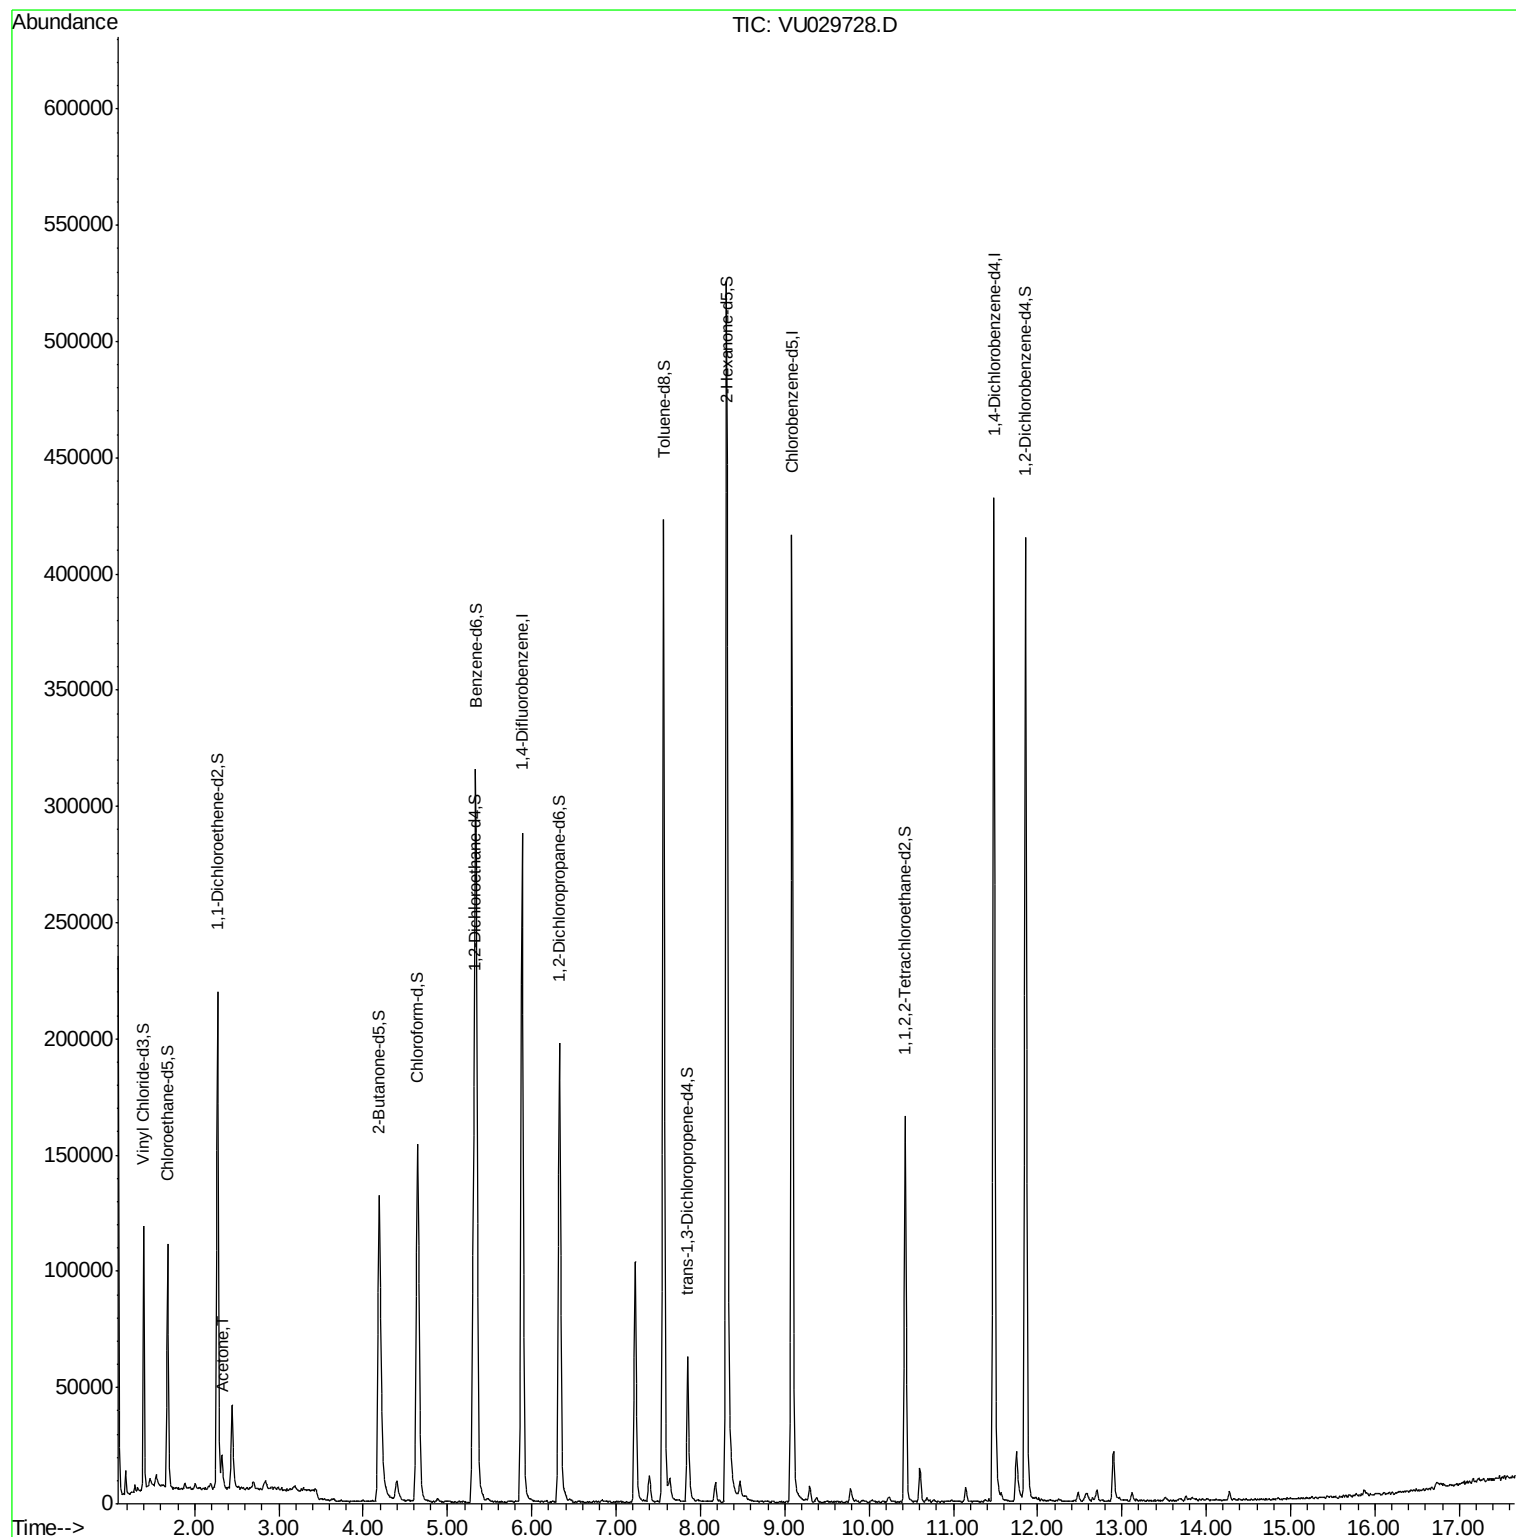

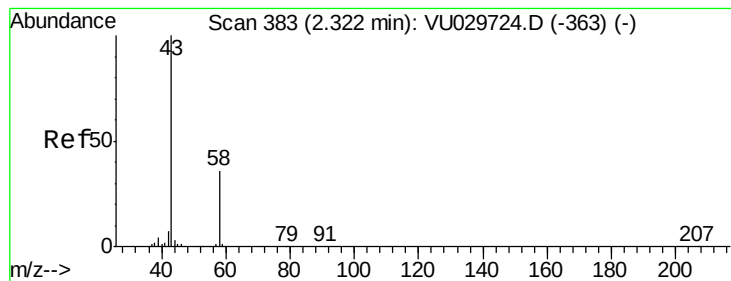

#13

Acetone

Concen: 4.697 ug/L

RT: 2.32 min Scan# 383

Delta R.T. -0.00 min

Lab File: VU029728.D

Acq: 28 Feb 2019 11:20

Instrument :

MSVOA_U

ClientSampleId :

CWK11

Tgt Ion: 43 Resp: 13015

Ion Ratio Lower Upper

43 100

58 37.9 0.0 70.2

