

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU022819\
 Data File : VU029729.D
 Acq On : 28 Feb 2019 11:43
 Operator : JC/SP
 Sample : K1577-19
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CWK08

Quant Time: Mar 01 00:38:54 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR022119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Mar 01 00:18:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	257176	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	244186	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	125614	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	73008	4.35	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.00%
7) Chloroethane-d5	1.68	69	70941	4.49	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.80%
11) 1,1-Dichloroethene-d2	2.27	63	114429	3.17	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.40%
20) 2-Butanone-d5	4.19	46	212181	55.88	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.76%
24) Chloroform-d	4.65	84	149926	5.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.40%
26) 1,2-Dichloroethane-d4	5.31	65	81589	5.10	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.00%
32) Benzene-d6	5.34	84	324784	5.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.60%
36) 1,2-Dichloropropane-d6	6.33	67	99230	5.44	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.80%
41) Toluene-d8	7.56	98	294996	4.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.20%
43) trans-1,3-Dichloropropene-	7.85	79	37345	4.99	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	99.80%
46) 2-Hexanone-d5	8.31	63	203796	55.53	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.06%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	82287	5.02	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.40%
64) 1,2-Dichlorobenzene-d4	11.86	152	125230	5.07	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.40%


Target Compounds					Qvalue
13) Acetone	2.33	43	13386	4.907 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU022819\
Data File : VU029729.D
Acq On : 28 Feb 2019 11:43
Operator : JC/SP
Sample : K1577-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CWK08

Quant Time: Mar 01 00:38:54 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR022119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Mar 01 00:18:18 2019
Response via : Initial Calibration

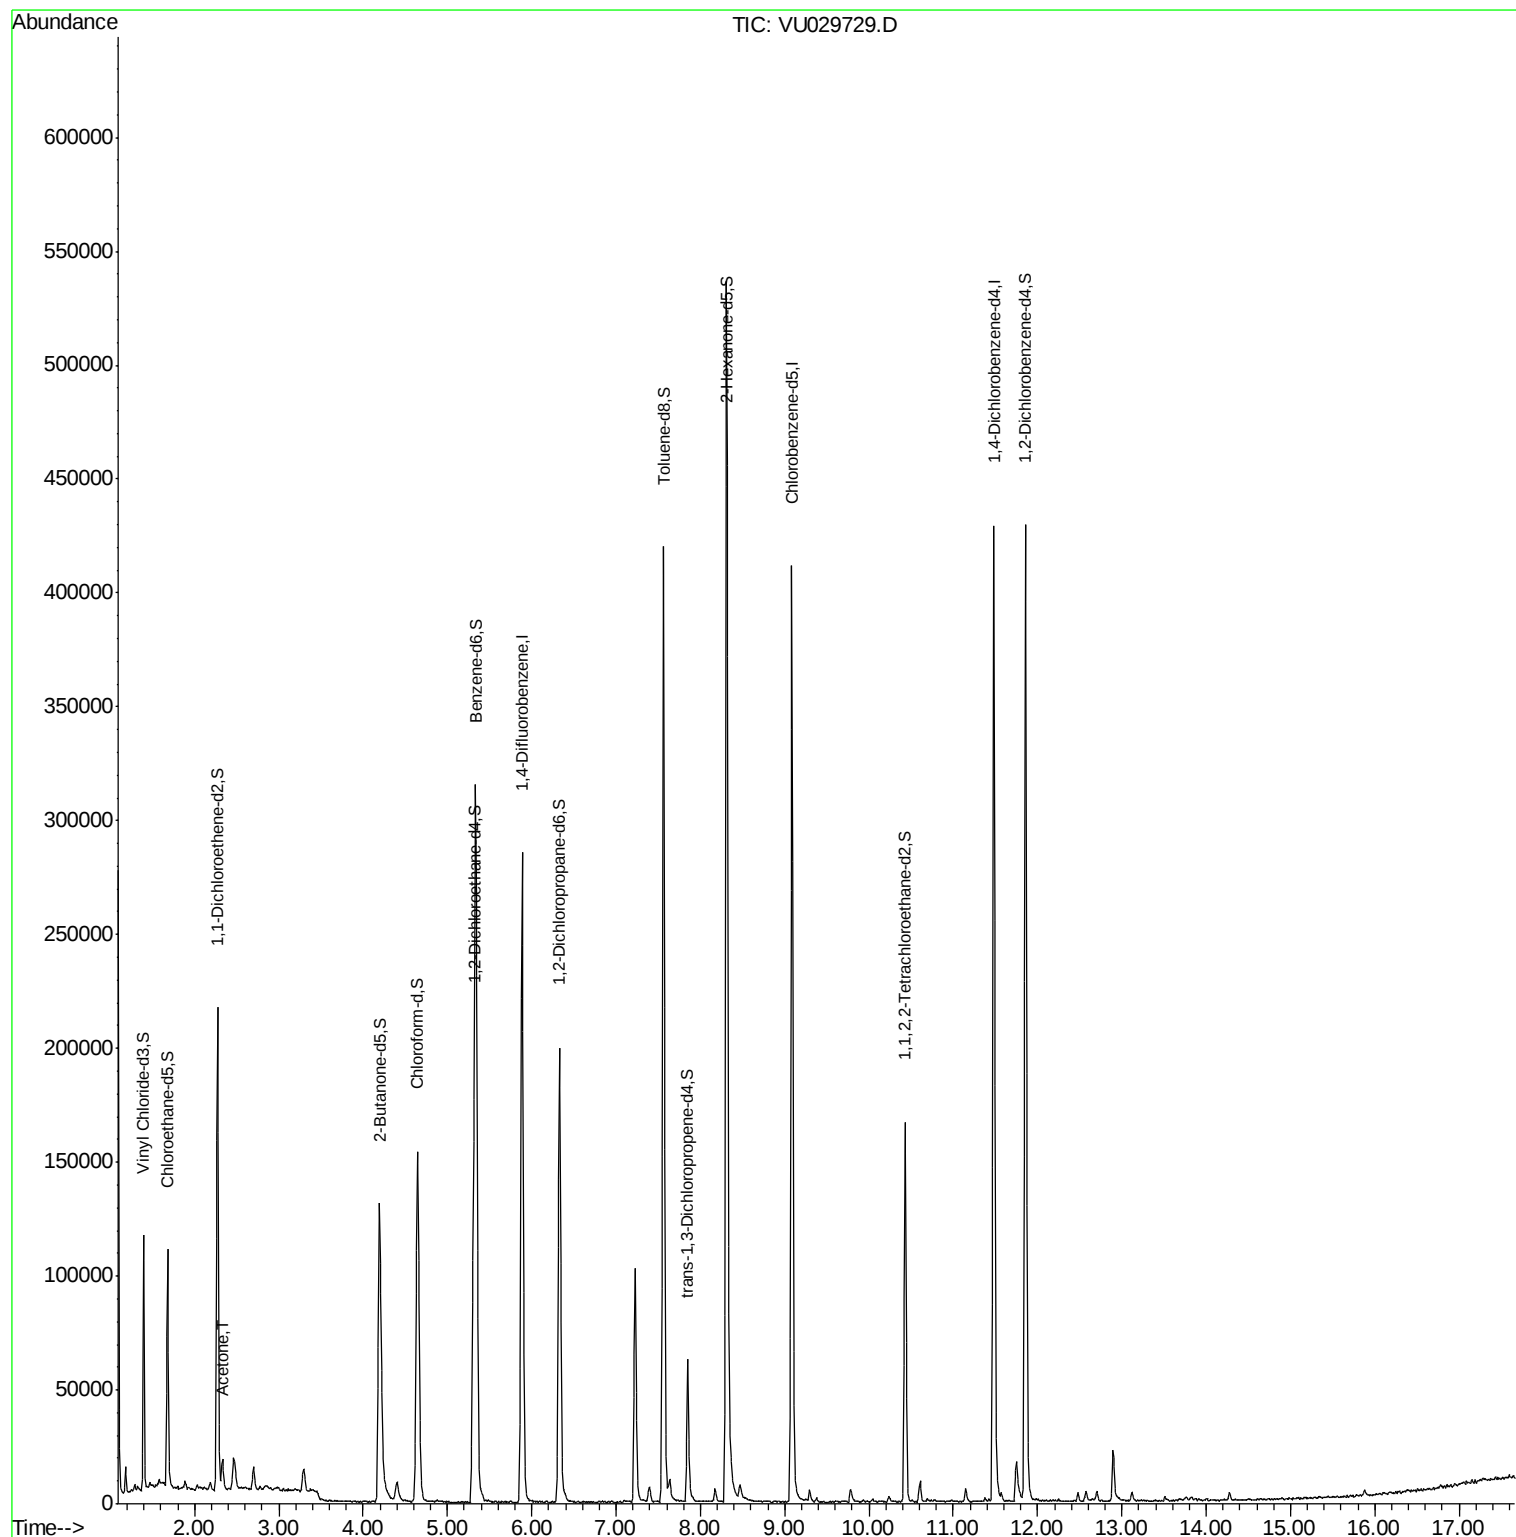

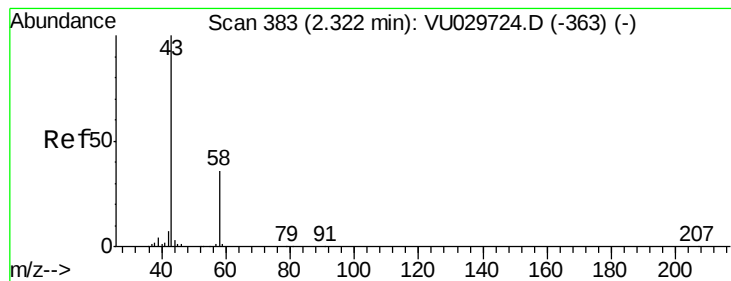

#13
 Acetone
 Concen: 4.907 ug/L
 RT: 2.33 min Scan# 385
 Delta R.T. 0.01 min
 Lab File: VU029729.D
 Acq: 28 Feb 2019 11:43

Instrument :
 MSVOA_U
 ClientSampleId :
 CWK08

Tgt Ion: 43 Resp: 13386
 Ion Ratio Lower Upper
 43 100
 58 33.6 0.0 70.2

