


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU022820\
 Data File : VU036959.D
 Acq On : 28 Feb 2020 09:06
 Operator : JC/MD
 Sample : BFB54
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB54

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
 Title : VOC Analysis
 Last Update : Sat Feb 29 00:30:49 2020

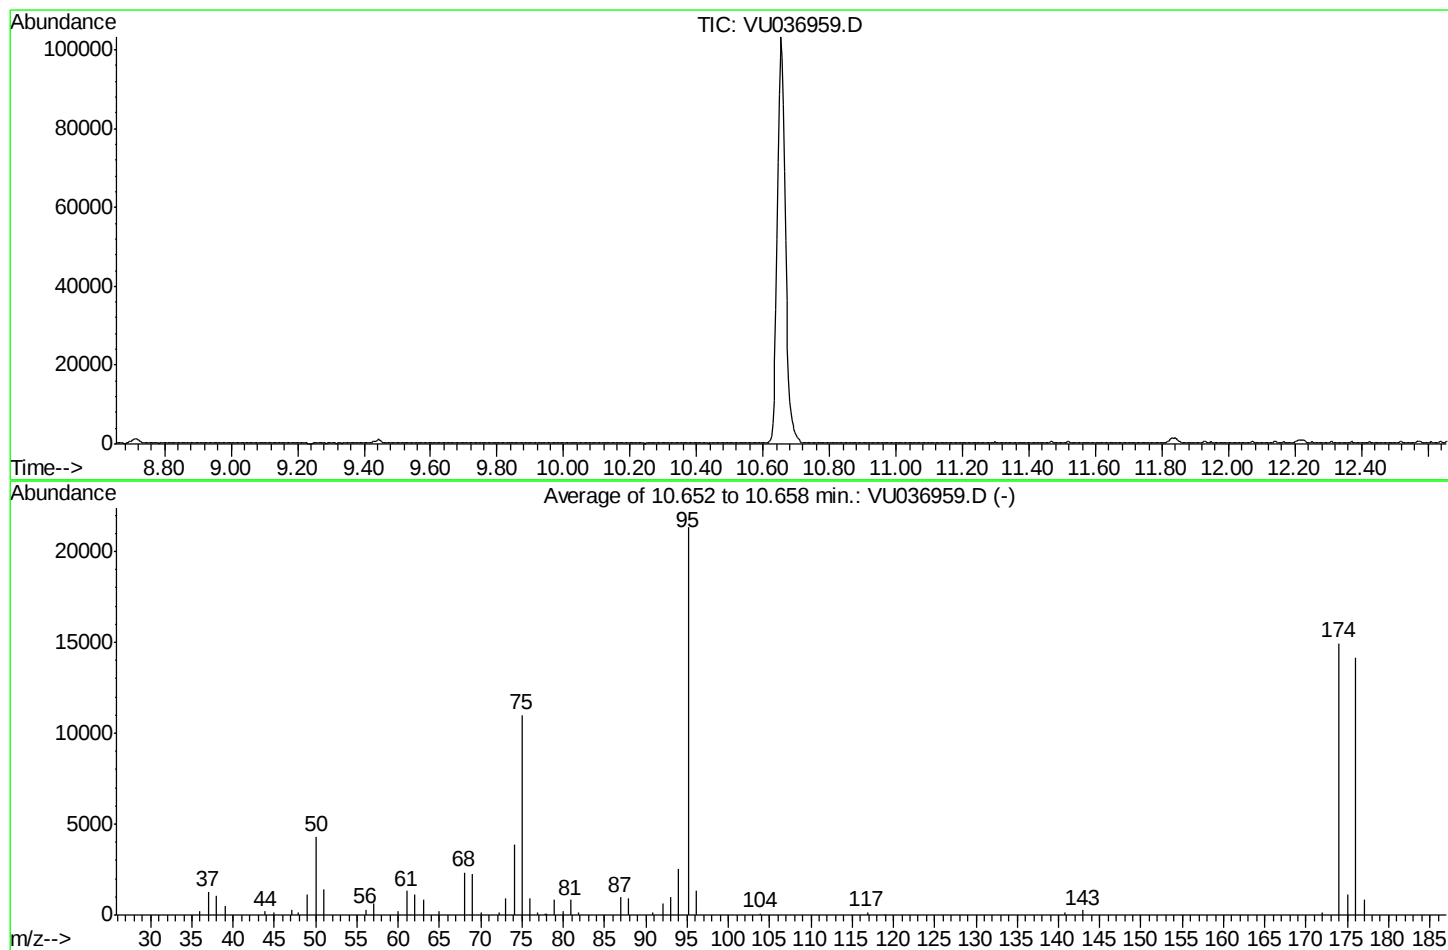

AutoFind: Scans 2896, 2897, 2898; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	4311	PASS
75	95	30	80	51.6	11003	PASS
95	95	100	100	100.0	21330	PASS
96	95	5	9	6.4	1362	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.0	14938	PASS
175	174	5	9	7.4	1105	PASS
176	174	95	101	95.0	14192	PASS
177	176	5	9	6.2	882	PASS

m/z	Abundance
35.90	218.0
37.00	1302.0
38.00	1122.0
39.00	516.0
44.00	481.0
45.00	178.0
47.10	311.0
47.90	145.0
49.00	1171.0
50.00	4434.0
51.00	1368.0
56.10	311.0
57.00	626.0
60.00	204.0
61.00	1315.0
62.10	1066.0
63.00	898.0
65.00	204.0
68.00	2379.0
69.00	2358.0
70.00	141.0
72.20	132.0
73.00	880.0
74.00	3983.0
75.00	10774.0
76.00	915.0
76.90	157.0
77.80	125.0
78.90	858.0
79.90	193.0
80.90	808.0
81.90	171.0
87.00	974.0
87.90	899.0
91.00	126.0
92.00	653.0
93.00	1003.0
94.00	2566.0
95.10	21440.0
96.10	1348.0
103.90	129.0
116.80	152.0
118.90	112.0
140.80	141.0
143.00	257.0
171.90	156.0
174.00	14334.0
175.10	1134.0
176.00	13794.0
177.00	772.0

Instrument :
MSVOA_U
ClientSampleId :
BFB54

m/z	Abundance
35.90	218.0
37.00	1294.0
38.00	1116.0
39.00	569.0
44.00	495.0
44.90	169.0
47.10	309.0
47.90	138.0
49.00	1148.0
50.00	4409.0
51.00	1416.0
56.00	301.0
56.90	638.0
59.90	221.0
61.00	1359.0
62.10	1148.0
63.00	858.0
65.00	221.0
68.00	2385.0
69.00	2305.0
70.00	137.0
72.20	125.0
73.00	885.0
74.00	4084.0
75.00	11384.0
76.00	971.0
76.90	190.0
78.00	113.0
78.90	868.0
79.90	223.0
80.90	846.0
81.90	186.0
87.00	966.0
87.90	935.0
90.90	108.0
92.00	705.0
93.00	1043.0
94.00	2595.0
95.10	21792.0
96.10	1373.0
103.90	119.0
116.90	184.0
140.80	150.0
143.00	265.0
171.90	147.0
174.00	15396.0
175.10	1125.0
176.00	14690.0
177.00	909.0

Instrument :
MSVOA_U
ClientSampleId :
BFB54

m/z	Abundance
35.90	178.0
37.00	1210.0
38.00	996.0
39.00	504.0
43.90	490.0
45.00	164.0
47.10	266.0
47.90	125.0
49.00	1002.0
50.10	4091.0
51.00	1348.0
56.00	298.0
56.90	602.0
59.90	229.0
61.00	1288.0
62.00	1095.0
63.00	839.0
65.00	198.0
68.00	2264.0
69.00	2064.0
70.00	147.0
72.10	115.0
73.00	907.0
74.10	3611.0
75.00	10853.0
76.00	947.0
76.90	182.0
78.00	111.0
78.90	841.0
79.90	220.0
80.90	795.0
81.90	174.0
86.90	950.0
87.90	856.0
90.80	102.0
92.00	649.0
93.00	978.0
94.00	2407.0
95.10	20760.0
96.10	1366.0
116.90	180.0
140.90	148.0
143.00	229.0
171.90	148.0
174.00	15086.0
175.00	1058.0
176.00	14093.0
177.00	967.0

Instrument :
MSVOA_U
ClientSampleId :
BFB54

Scan 2884 (10.613 min): VU036959.D
BFB54

m/z	Abundance
39.90	117.0
43.90	304.0

Instrument :
MSVOA_U
ClientSampleId :
BFB54