

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022823\
 Data File : VU053164.D
 Acq On : 28 Feb 2023 10:36
 Operator : JC/MD
 Sample : VU0228WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0228WBL01

Quant Time: Mar 01 03:37:06 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U022723DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Feb 28 03:35:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.112	96	25278	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.633	95	10440	0.979	ug/l	0.00
Spiked Amount 1.000			Recovery	=	98.000%	
68) 1,2-Dichlorobenzene-d4	12.193	152	8181	0.967	ug/l	0.00
Spiked Amount 1.000			Recovery	=	97.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022823\
Data File : VU053164.D
Acq On : 28 Feb 2023 10:36
Operator : JC/MD
Sample : VU0228WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0228WBL01

Quant Time: Mar 01 03:37:06 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U022723DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Feb 28 03:35:42 2023
Response via : Initial Calibration




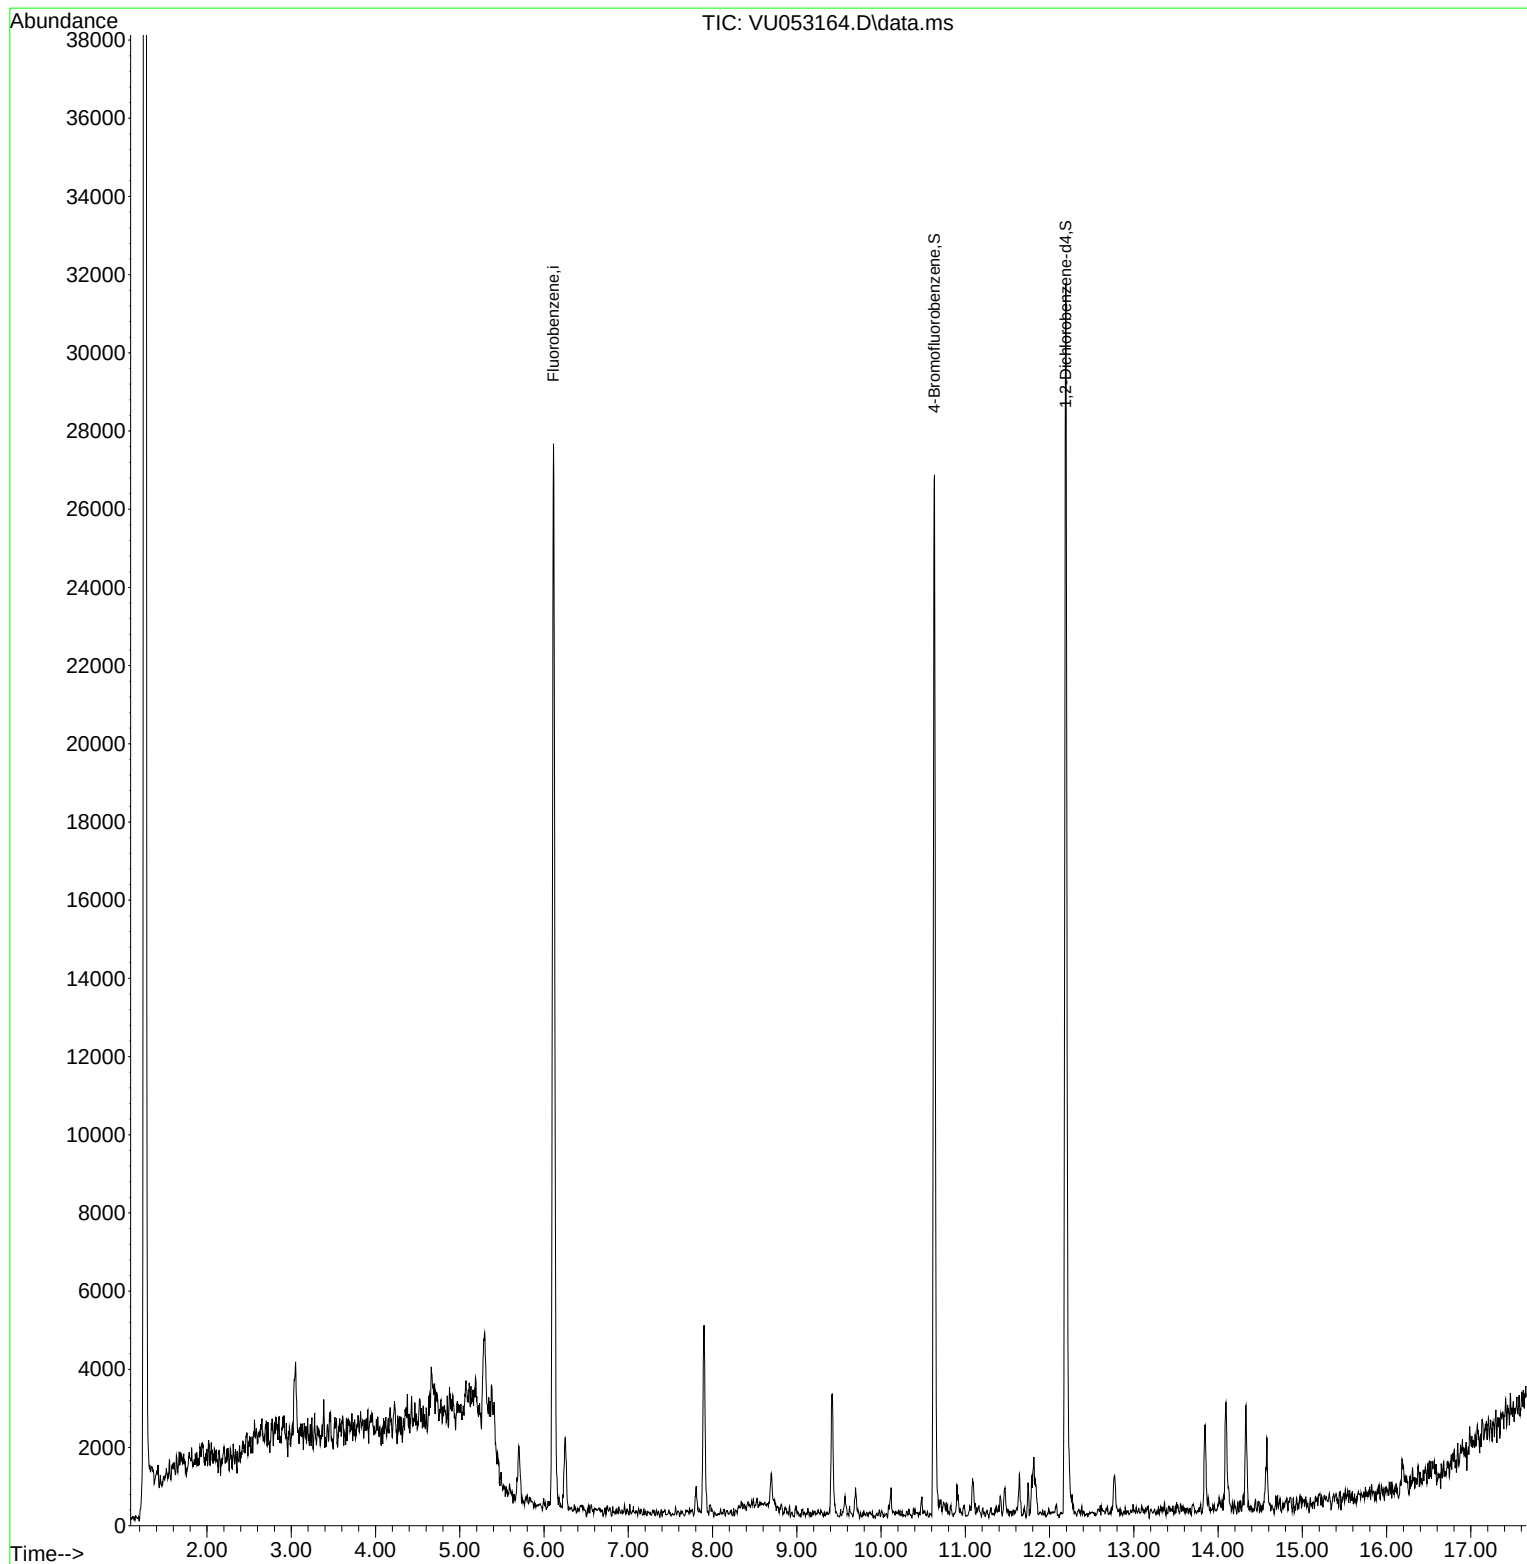


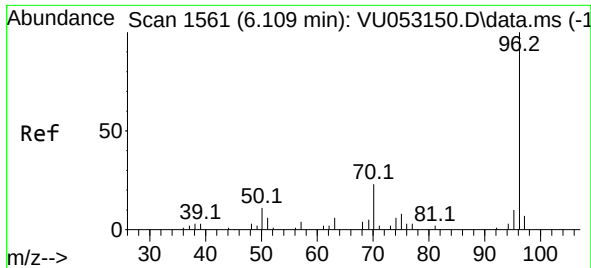

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.112 min Scan# 1
Delta R.T. 0.003 min
Lab File: VU053164.D
Acq: 28 Feb 2023 10:36




Instrument :
MSVOA_U
ClientSampleId :
VU0228WBL01


Tgt Ion: 96	Resp: 25278
Ion Ratio	Lower Upper
96 100	
70 21.4	15.5 23.3
95 8.9	7.0 10.6
97 5.9	0.0 0.0#

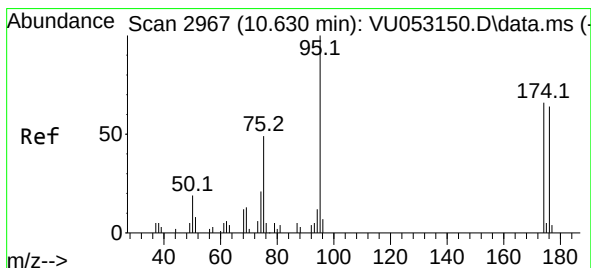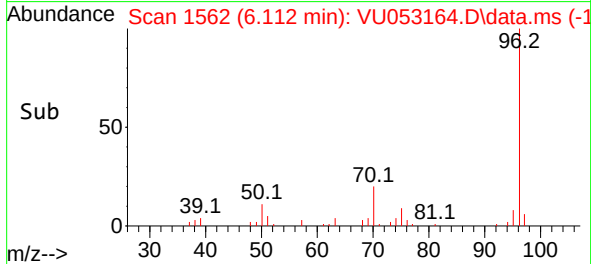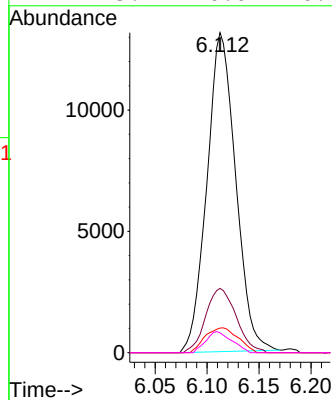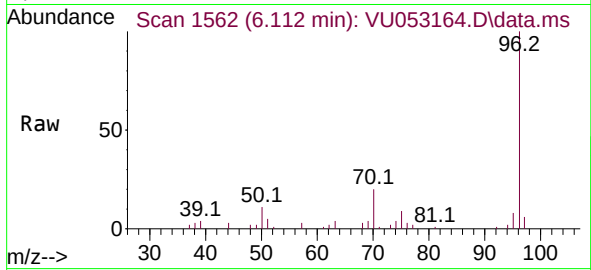

#57
4-Bromofluorobenzene
Concen: 0.979 ug/l
RT: 10.633 min Scan# 2968
Delta R.T. 0.003 min
Lab File: VU053164.D
Acq: 28 Feb 2023 10:36


Tgt Ion: 95	Resp: 10440
Ion Ratio	Lower Upper
95 100	
174 64.0	50.7 76.1
176 58.4	47.8 71.6

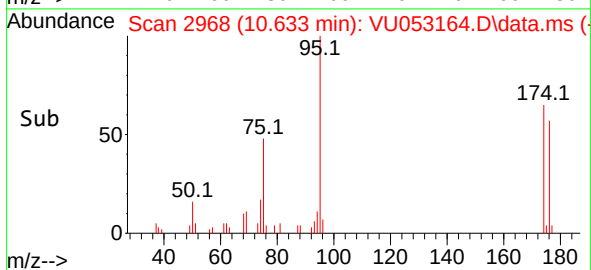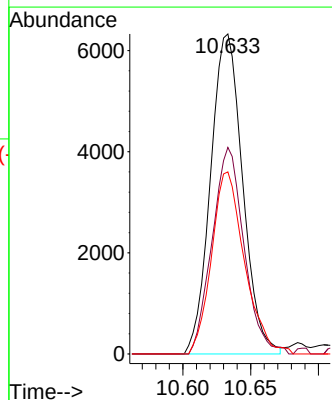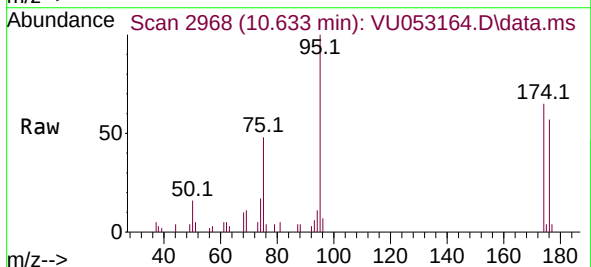

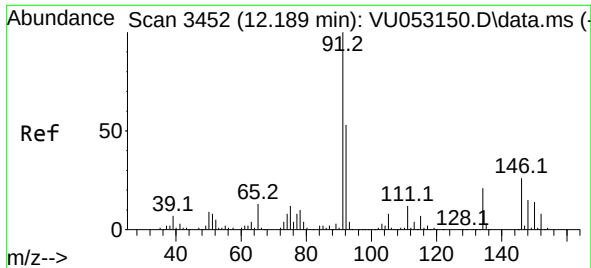

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.967 ug/l
 RT: 12.193 min Scan# 3453
 Delta R.T. 0.003 min
 Lab File: VU053164.D
 Acq: 28 Feb 2023 10:36

Instrument : MSVOA_U
 ClientSampleId : VU0228WBL01

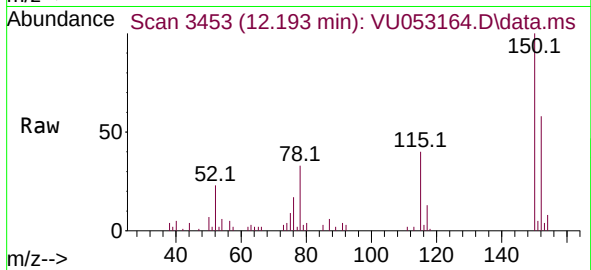

Tgt Ion:	152	Resp:	8181
Ion Ratio	Lower	Upper	
152	100		
115	70.0	0.0	267.8
150	165.5	0.0	623.0

