

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022823\
 Data File : VU053167.D
 Acq On : 28 Feb 2023 12:13
 Operator : JC/MD
 Sample : BLK
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BLK

Quant Time: Mar 01 03:38:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U022723DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Feb 28 03:35:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	0.000	96	0	0.000	ug/l	-6.11
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.633	95	545	0.000	ug/l	0.00
Spiked Amount 1.000			Recovery	=	0.000%	
68) 1,2-Dichlorobenzene-d4	0.000	152	0	0.000	ug/l	
Spiked Amount 1.000			Recovery	=	0.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022823\
Data File : VU053167.D
Acq On : 28 Feb 2023 12:13
Operator : JC/MD
Sample : BLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BLK

Quant Time: Mar 01 03:38:59 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U022723DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Feb 28 03:35:42 2023
Response via : Initial Calibration

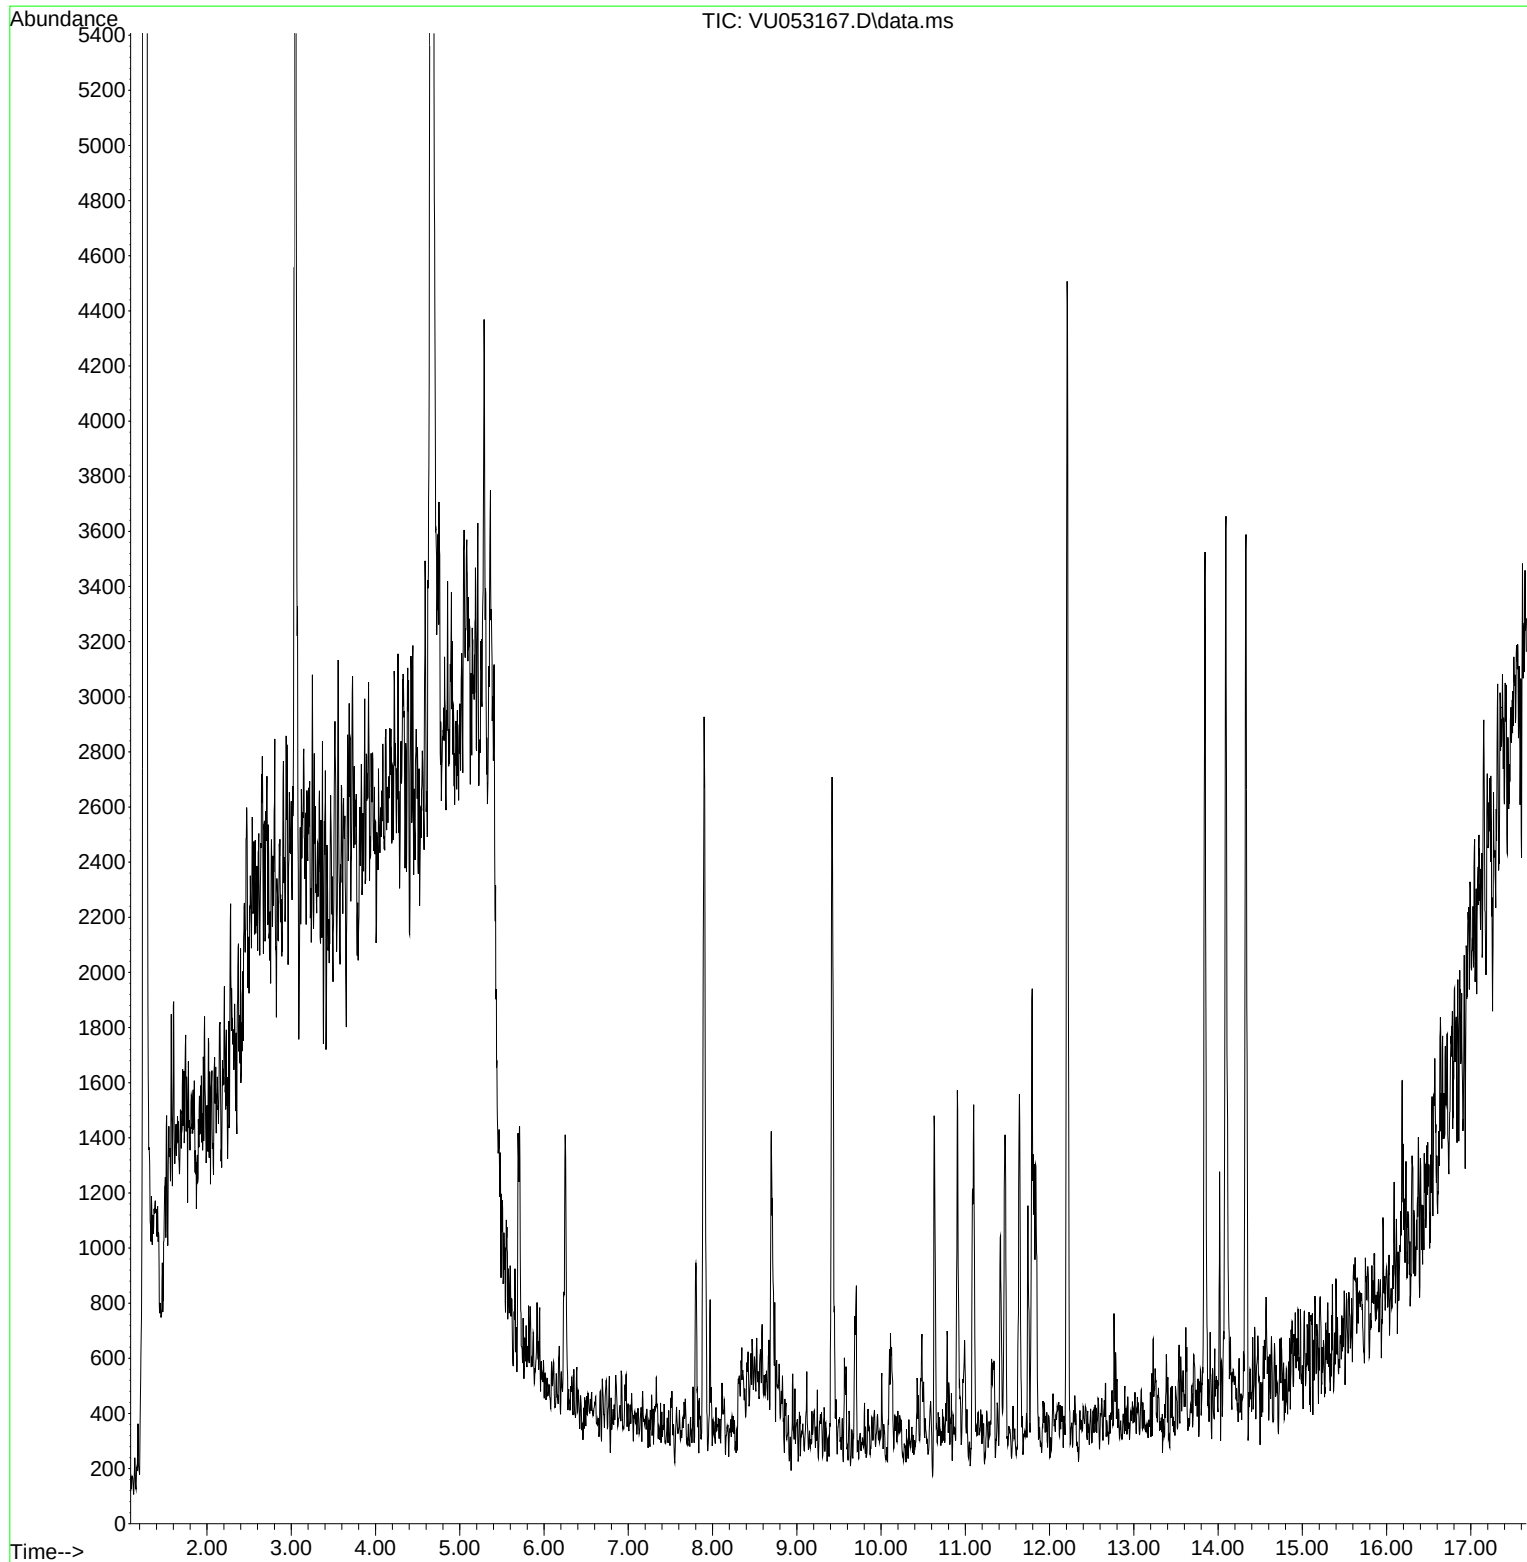


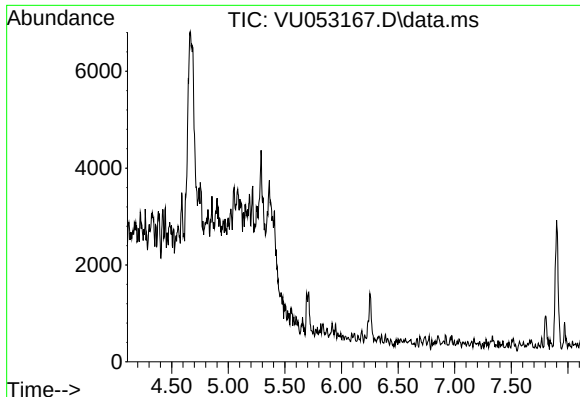


#1
Fluorobenzene
Concen: 0.000 ug/l
Expected RT: 6.11 min

Lab File: VU053167.D
Acq: 28 Feb 2023 12:13




Instrument :
MSVOA_U
ClientSampleId :
BLK


Tgt Ion: 96
Sig Exp Ratio
96 100
70 19.4
95 8.8
97 0.0

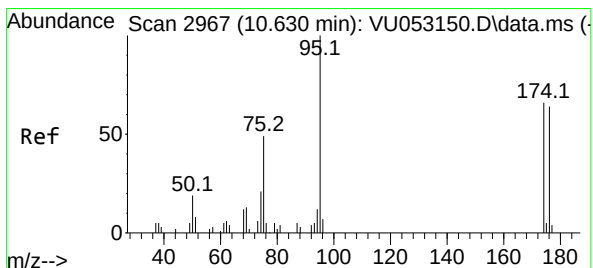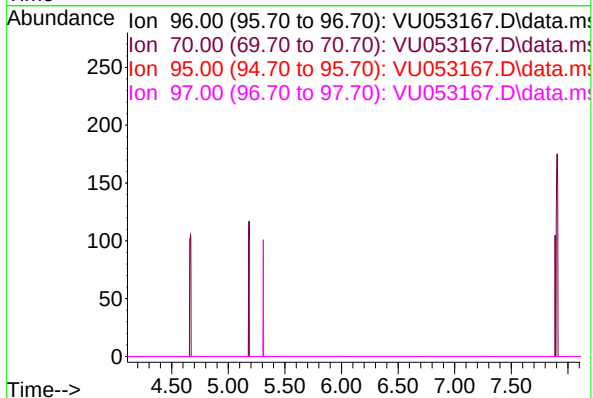

#57
4-Bromofluorobenzene
Concen: 0.000 ug/l
RT: 10.633 min Scan# 2968
Delta R.T. 0.003 min
Lab File: VU053167.D
Acq: 28 Feb 2023 12:13

Tgt Ion: 95 Resp: 545
Ion Ratio Lower Upper
95 100
174 48.6 50.7 76.1#
176 50.6 47.8 71.6

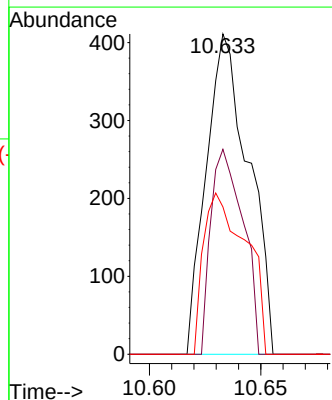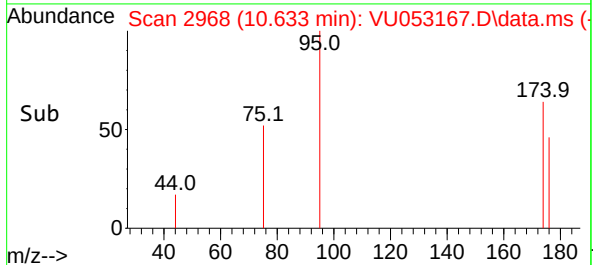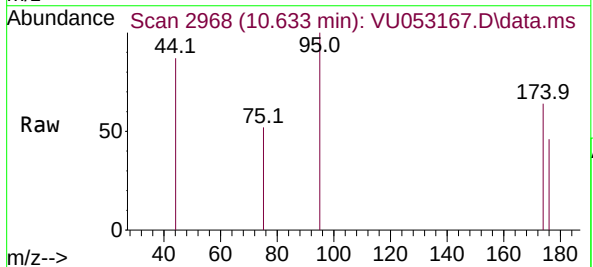

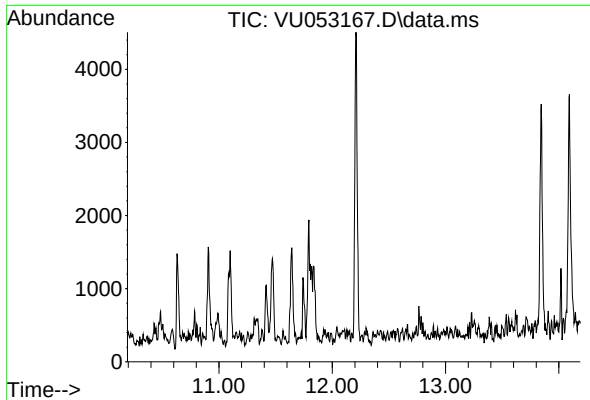

#68
1,2-Dichlorobenzene-d4
Concen: 0.000 ug/l
Expected RT: 12.19 min
Lab File: VU053167.D
Acq: 28 Feb 2023 12:13

Instrument :
MSVOA_U
ClientSampleId :
BLK

Tgt Ion: 152
Sig Exp Ratio
152 100
115 133.9
150 311.5

