

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022823\
 Data File : VU053164.D
 Acq On : 28 Feb 2023 10:36
 Operator : JC/MD
 Sample : VU0228WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0228WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U022723DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU053164.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.945	262	266	273	rVB5	533	651	1.16%	0.294%
2	2.142	324	327	333	rVB5	655	648	1.16%	0.292%
3	2.277	365	369	373	rVV4	595	640	1.14%	0.289%
4	2.312	377	380	385	rVV2	736	672	1.20%	0.303%
5	2.338	385	388	394	rVB3	618	610	1.09%	0.275%
6	2.762	515	520	522	rBV2	765	637	1.14%	0.287%
7	2.855	545	549	552	rVB2	676	561	1.00%	0.253%
8	2.942	574	576	581	rVB2	871	582	1.04%	0.262%
9	2.977	581	587	592	rBV3	783	1066	1.90%	0.481%
10	3.051	600	610	619	rBV6	1884	3544	6.33%	1.598%
11	3.154	639	642	646	rBV5	686	641	1.14%	0.289%
12	3.244	667	670	675	rVB3	812	626	1.12%	0.282%
13	3.277	678	680	687	rVB4	827	563	1.01%	0.254%
14	3.386	710	714	718	rVB4	1238	995	1.78%	0.449%
15	3.518	749	755	756	rBV2	822	733	1.31%	0.331%
16	3.576	765	773	775	rBV5	728	845	1.51%	0.381%
17	3.939	880	886	888	rBV4	648	822	1.47%	0.371%
18	4.174	955	959	962	rBV3	663	668	1.19%	0.301%
19	4.662	1108	1111	1116	rBV3	1050	1184	2.11%	0.534%
20	4.878	1175	1178	1180	rBV3	951	644	1.15%	0.290%
21	5.286	1296	1305	1306	rBV4	2319	2933	5.24%	1.323%
22	5.376	1330	1333	1339	rBV4	803	795	1.42%	0.359%
23	5.701	1429	1434	1444	rVB4	1469	2597	4.64%	1.171%
24	6.112	1549	1562	1580	rVB	27140	51791	92.51%	23.358%
25	6.251	1598	1605	1617	rVB2	1849	3400	6.07%	1.533%
26	7.807	2079	2089	2099	rBV4	768	1240	2.21%	0.559%
27	7.900	2107	2118	2130	rBV	4803	8337	14.89%	3.760%
28	8.698	2359	2366	2375	rBV4	769	1143	2.04%	0.515%
29	9.421	2582	2591	2603	rVB4	3032	5250	9.38%	2.368%
30	9.572	2631	2638	2646	rVB2	469	698	1.25%	0.315%
31	9.697	2667	2677	2684	rBV2	743	1114	1.99%	0.502%
32	10.633	2958	2968	2983	rBV2	26630	43846	78.32%	19.775%
33	10.900	3042	3051	3054	rBV3	752	673	1.20%	0.304%
34	11.086	3103	3109	3111	rBV2	816	781	1.40%	0.352%
35	11.414	3207	3211	3218	rVB3	504	597	1.07%	0.269%
36	11.472	3218	3229	3235	rBV3	715	1180	2.11%	0.532%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022823\
 Data File : VU053164.D
 Acq On : 28 Feb 2023 10:36
 Operator : JC/MD
 Sample : VU0228WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0228WBL01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U022723DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER

37	11.643	3275	3282	3286	rBV2	938	1050	1.88%	0.474%
38	11.746	3306	3314	3318	rBV3	895	923	1.65%	0.416%
39	11.791	3322	3328	3330	rBV2	941	943	1.68%	0.425%
40	11.813	3330	3335	3338	rVV2	791	811	1.45%	0.366%
41	12.193	3442	3453	3474	rBV3	31458	55984	100.00%	25.249%
42	12.771	3625	3633	3640	rBV2	895	1518	2.71%	0.685%
43	13.848	3954	3968	3977	rBV4	2271	3967	7.09%	1.789%
44	14.093	4038	4044	4052	rBV3	2484	3746	6.69%	1.689%
45	14.331	4111	4118	4126	rVB5	2634	3824	6.83%	1.725%
46	14.578	4192	4195	4205	rVB3	1718	1639	2.93%	0.739%
47	15.372	4432	4442	4445	rBV3	404	619	1.11%	0.279%
48	15.665	4525	4533	4541	rBV3	317	680	1.21%	0.307%
49	16.971	4933	4939	4941	rBV3	616	694	1.24%	0.313%
50	16.987	4941	4944	4950	rVV5	729	711	1.27%	0.321%
51	17.134	4986	4990	4996	rBV6	704	914	1.63%	0.412%




Sum of corrected areas: 221730

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022823\
Data File : VU053164.D
Acq On : 28 Feb 2023 10:36
Operator : JC/MD
Sample : VU0228WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0228WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U022723DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

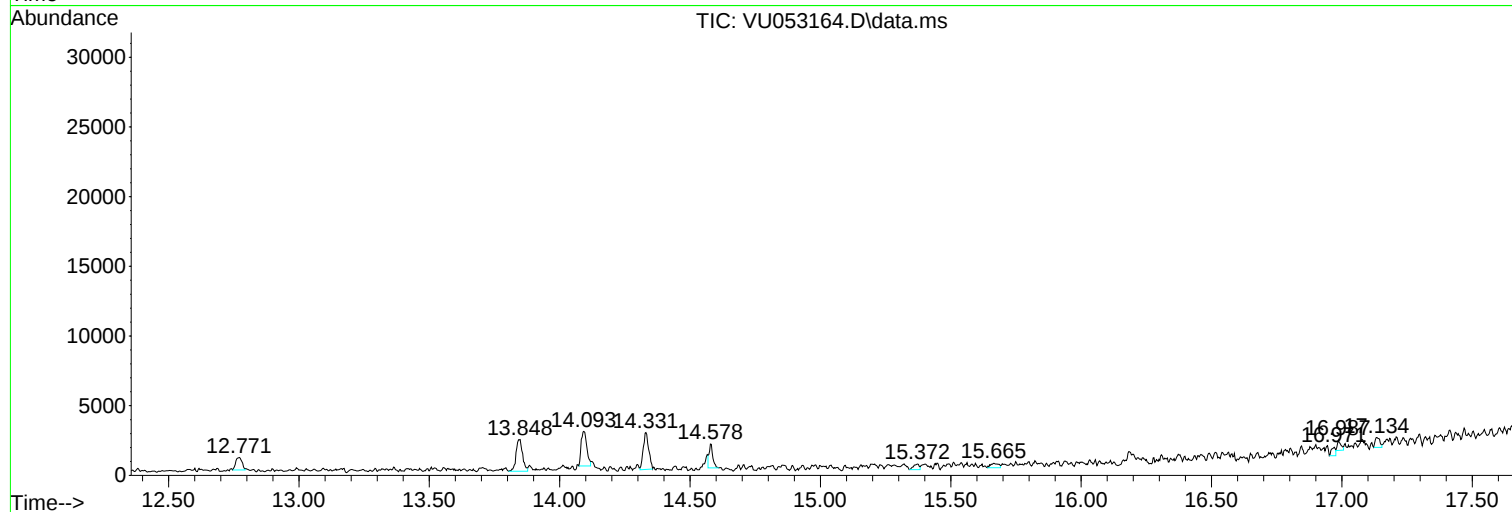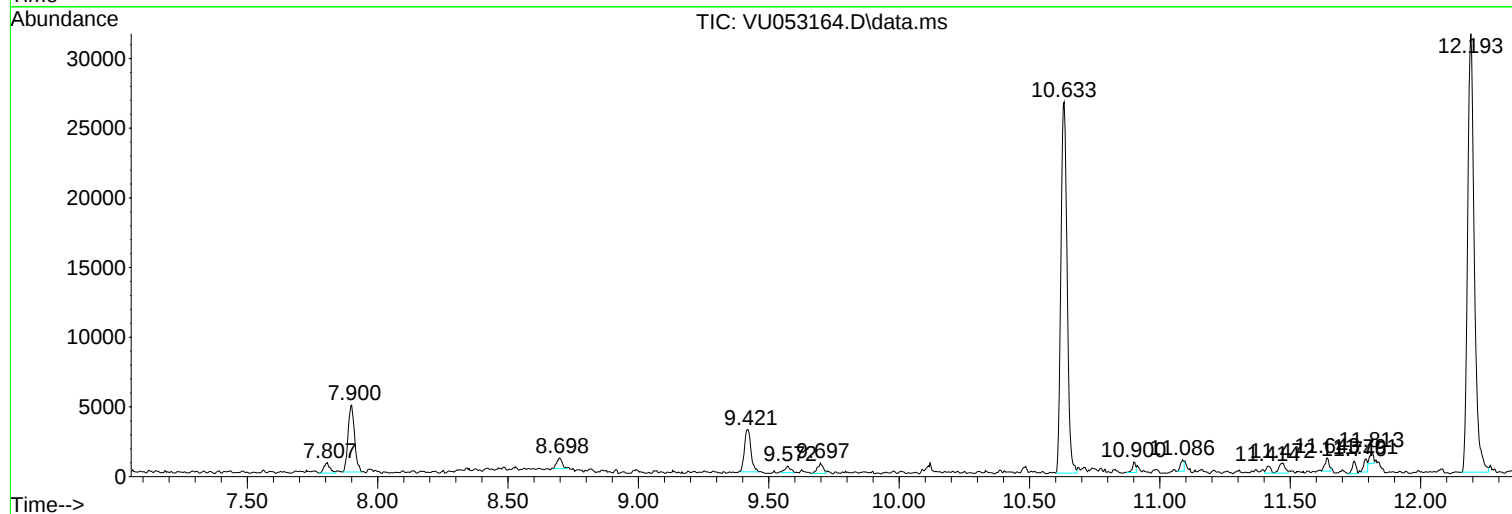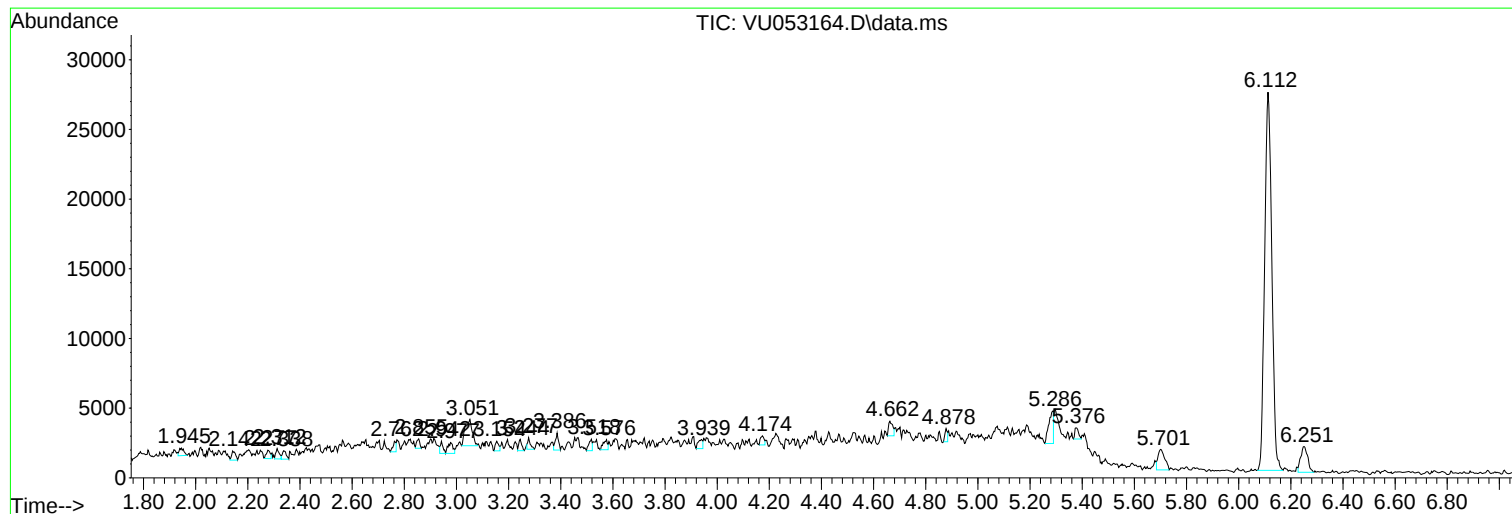

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022823\
Data File : VU053164.D
Acq On : 28 Feb 2023 10:36
Operator : JC/MD
Sample : VU0228WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0228WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U022723DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022823\
Data File : VU053164.D
Acq On : 28 Feb 2023 10:36
Operator : JC/MD
Sample : VU0228WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0228WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U022723DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc