


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022823\
Data File : VU053162.D
Acq On : 28 Feb 2023 08:59
Operator : JC/MD
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U022723DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Tue Feb 28 03:35:42 2023

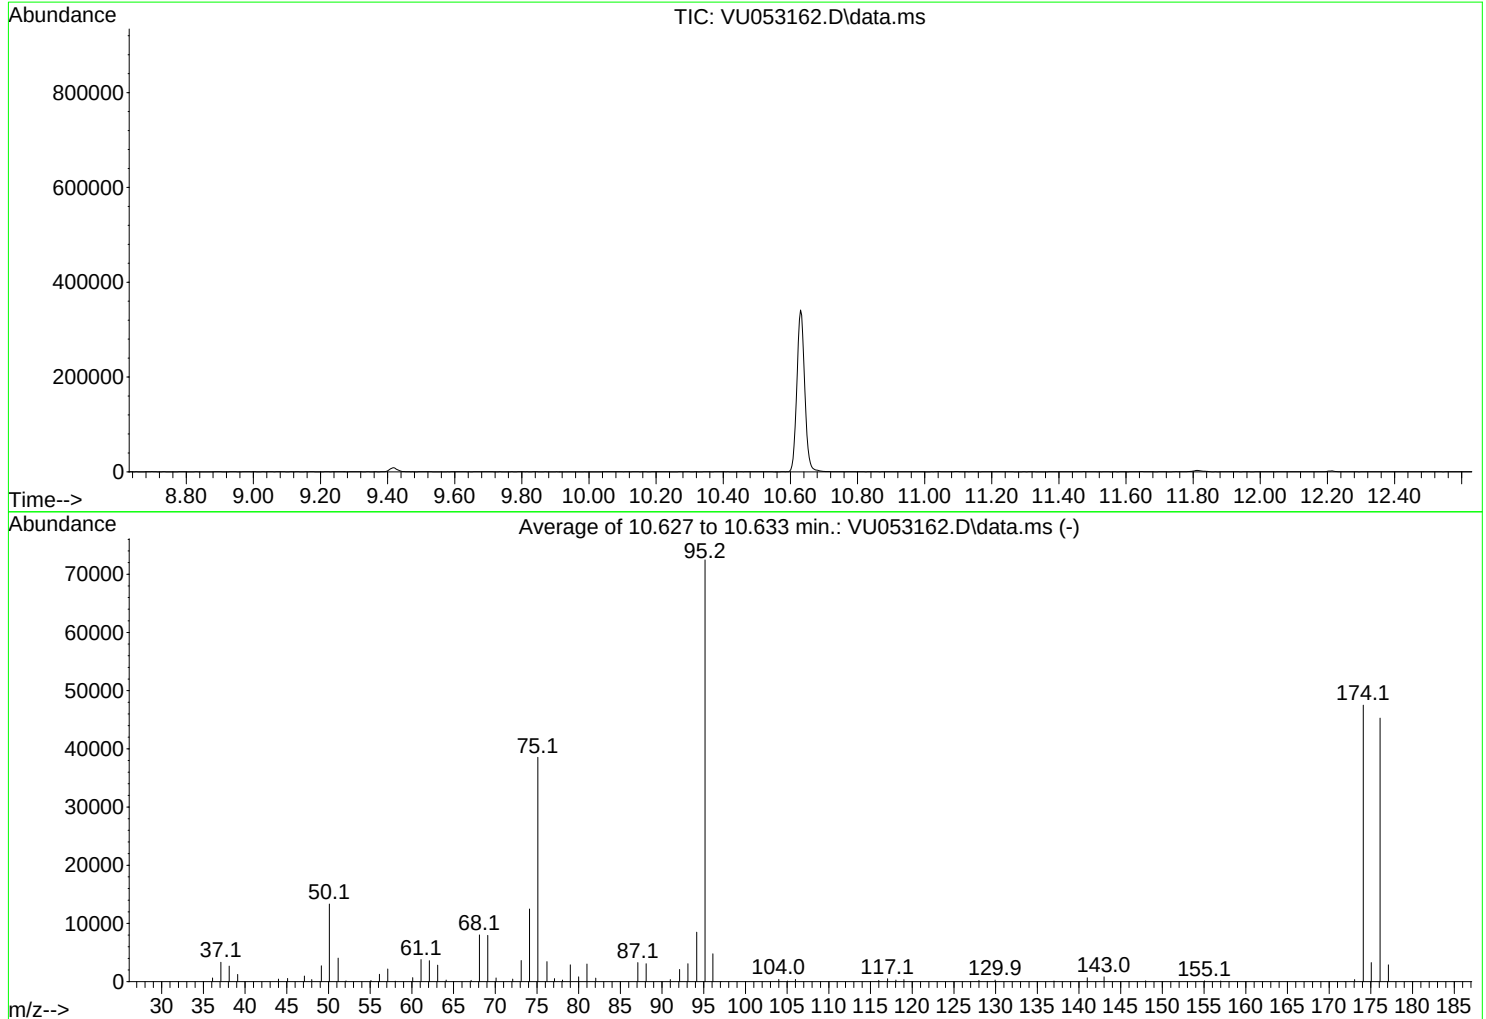

AutoFind: Scans 2966, 2967, 2968; Background Corrected with Scan 2953

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	13332	PASS
75	95	30	60	53.2	38533	PASS
95	95	100	100	100.0	72477	PASS
96	95	5	9	6.6	4774	PASS
173	174	0.00	2	0.8	373	PASS
174	95	50	100	65.6	47515	PASS
175	174	5	9	6.9	3277	PASS
176	174	95	101	95.3	45269	PASS
177	176	5	9	6.4	2881	PASS