


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022824\
Data File : VU057955.D
Acq On : 28 Feb 2024 09:01
Operator : MD/SY
Sample : BFB045
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB045

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Title : VOC Analysis
Last Update : Thu Feb 29 00:08:26 2024

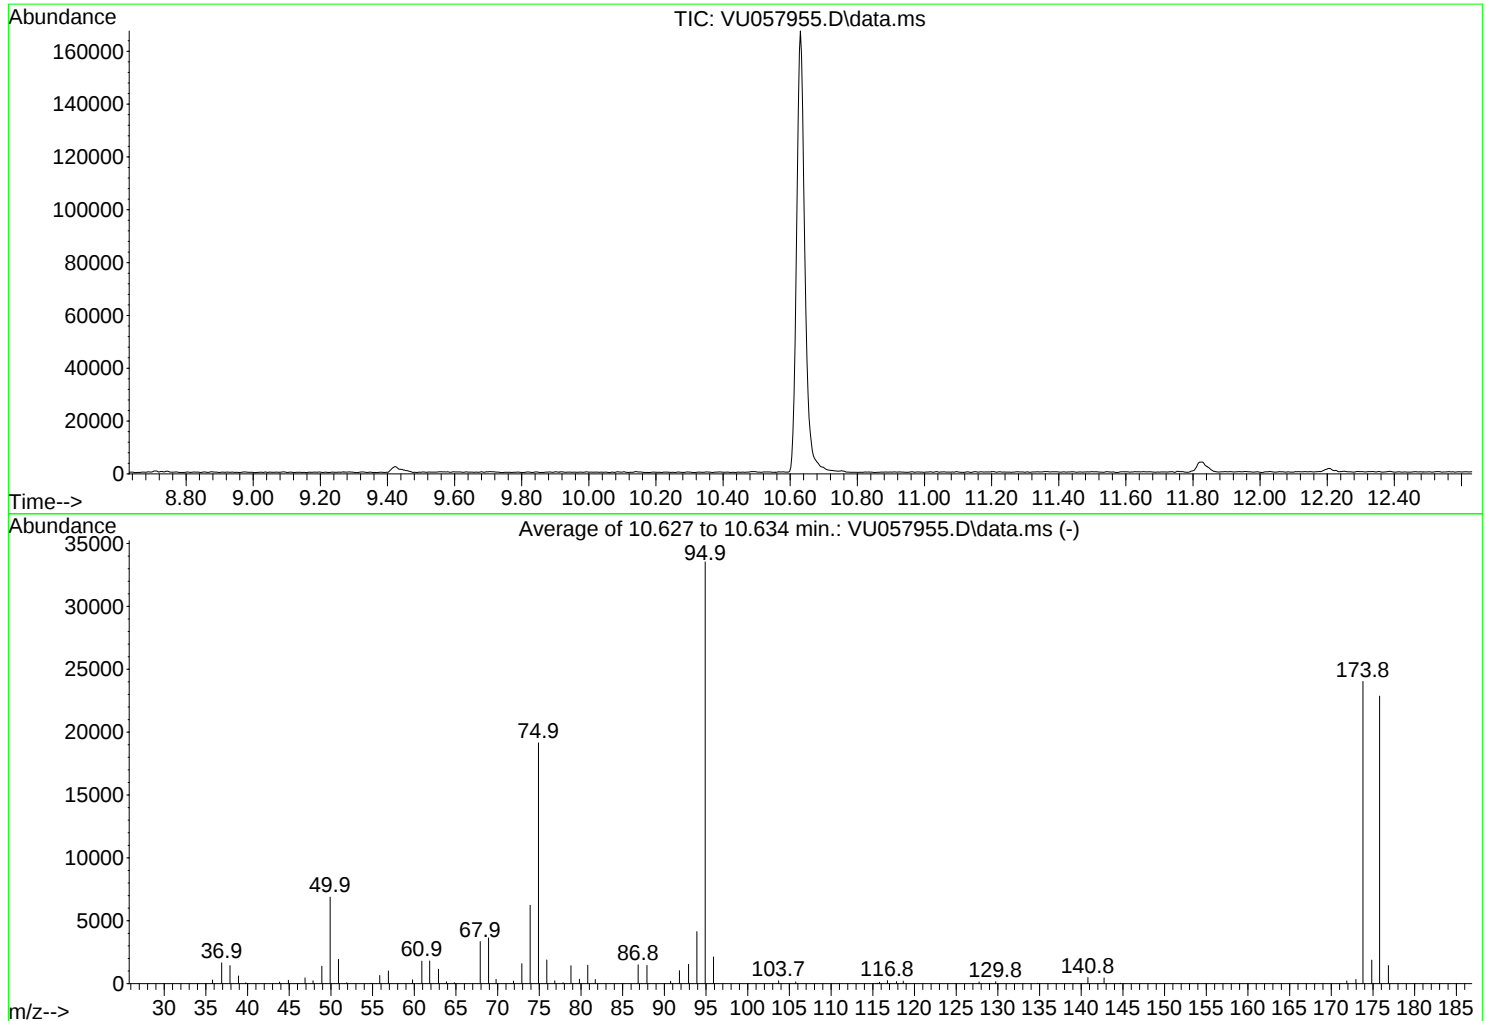

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2893

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	6891	PASS
75	95	30	80	57.1	19149	PASS
95	95	100	100	100.0	33544	PASS
96	95	5	9	6.3	2124	PASS
173	174	0.00	2	1.4	341	PASS
174	95	50	120	71.7	24035	PASS
175	174	5	9	7.8	1875	PASS
176	174	95	101	95.1	22867	PASS
177	176	5	9	6.3	1435	PASS

m/z	Abundance
39.80	260.0
43.80	423.0

Instrument :
MSVOA_U
ClientSampleId :
BFB045

m/z	Abundance
35.90	298.0
36.90	1743.0
37.90	1500.0
38.90	676.0
39.80	369.0
43.90	532.0
44.90	268.0
46.90	466.0
47.80	231.0
48.90	1452.0
49.90	6862.0
50.90	1845.0
55.80	637.0
56.90	966.0
59.80	276.0
60.90	1968.0
61.90	1854.0
62.90	1080.0
63.80	149.0
67.90	3414.0
68.90	3755.0
69.80	398.0
71.90	209.0
72.90	1602.0
73.90	5981.0
74.90	18976.0
75.90	1925.0
76.90	273.0
78.80	1380.0
79.80	337.0
80.80	1471.0
81.70	333.0
86.80	1555.0
87.90	1397.0
90.80	179.0
91.80	1055.0
92.90	1511.0
93.90	4052.0
94.90	33648.0
95.90	2151.0
103.70	269.0
105.70	145.0
115.60	135.0
116.80	248.0
117.80	139.0
118.60	198.0
127.70	125.0
129.80	154.0
140.80	529.0
142.70	458.0
171.90	178.0
173.00	330.0
173.80	23336.0
174.90	1871.0
175.80	21976.0
176.90	1336.0

Instrument :
MSVOA_U
ClientSampleId :
BFB045

m/z	Abundance
35.80	290.0
36.90	1718.0
37.90	1462.0
38.90	628.0
39.80	340.0
43.90	560.0
44.90	275.0
46.90	484.0
47.90	237.0
48.90	1400.0
49.90	7124.0
50.90	2011.0
51.90	111.0
55.90	652.0
56.90	1037.0
59.80	332.0
60.90	1843.0
61.80	1869.0
62.90	1153.0
63.80	151.0
64.80	108.0
67.90	3466.0
68.90	3774.0
69.80	365.0
71.90	210.0
72.90	1623.0
73.90	6436.0
74.90	19832.0
75.90	1980.0
76.80	239.0
77.80	114.0
78.80	1474.0
79.80	352.0
80.80	1487.0
81.70	349.0
86.80	1550.0
87.90	1521.0
90.70	185.0
91.80	1081.0
92.90	1597.0
93.90	4306.0
94.90	34616.0
95.90	2188.0
103.70	240.0
105.80	151.0
115.80	154.0
116.80	242.0
117.90	169.0
118.70	220.0
127.80	147.0
129.80	177.0
140.80	505.0
142.80	478.0
144.70	103.0
171.80	205.0
173.00	357.0
173.80	24936.0
174.80	1928.0
175.80	23680.0
176.90	1440.0

Instrument :
MSVOA_U
ClientSampleId :
BFB045

m/z	Abundance
35.70	286.0
36.90	1491.0
37.90	1348.0
38.90	542.0
39.80	302.0
43.90	556.0
44.90	276.0
46.90	434.0
47.90	232.0
48.90	1300.0
49.90	6686.0
50.90	1955.0
51.90	130.0
54.80	110.0
55.90	671.0
56.90	1003.0
59.80	302.0
60.90	1559.0
61.80	1695.0
62.90	1221.0
63.90	166.0
64.80	124.0
67.90	3167.0
68.90	3380.0
69.80	283.0
71.90	203.0
72.90	1558.0
73.90	6290.0
74.90	18640.0
75.90	1734.0
76.80	182.0
77.90	109.0
78.80	1418.0
79.80	371.0
80.80	1421.0
81.70	330.0
86.90	1390.0
87.90	1453.0
90.80	193.0
91.80	968.0
92.90	1524.0
93.90	4062.0
94.90	32368.0
95.90	2032.0
103.70	182.0
105.80	143.0
115.80	179.0
116.70	232.0
117.80	186.0
118.70	208.0
127.70	153.0
129.70	156.0
134.80	109.0
140.80	421.0
142.80	443.0
171.80	281.0
172.90	337.0
173.80	23832.0
174.80	1827.0
175.80	22944.0
176.80	1529.0

Instrument :
MSVOA_U
ClientSampleId :
BFB045