


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022924\
Data File : VU057964.D
Acq On : 29 Feb 2024 08:36
Operator : MD/SY
Sample : BFB115
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB115

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Mar 01 05:18:22 2024

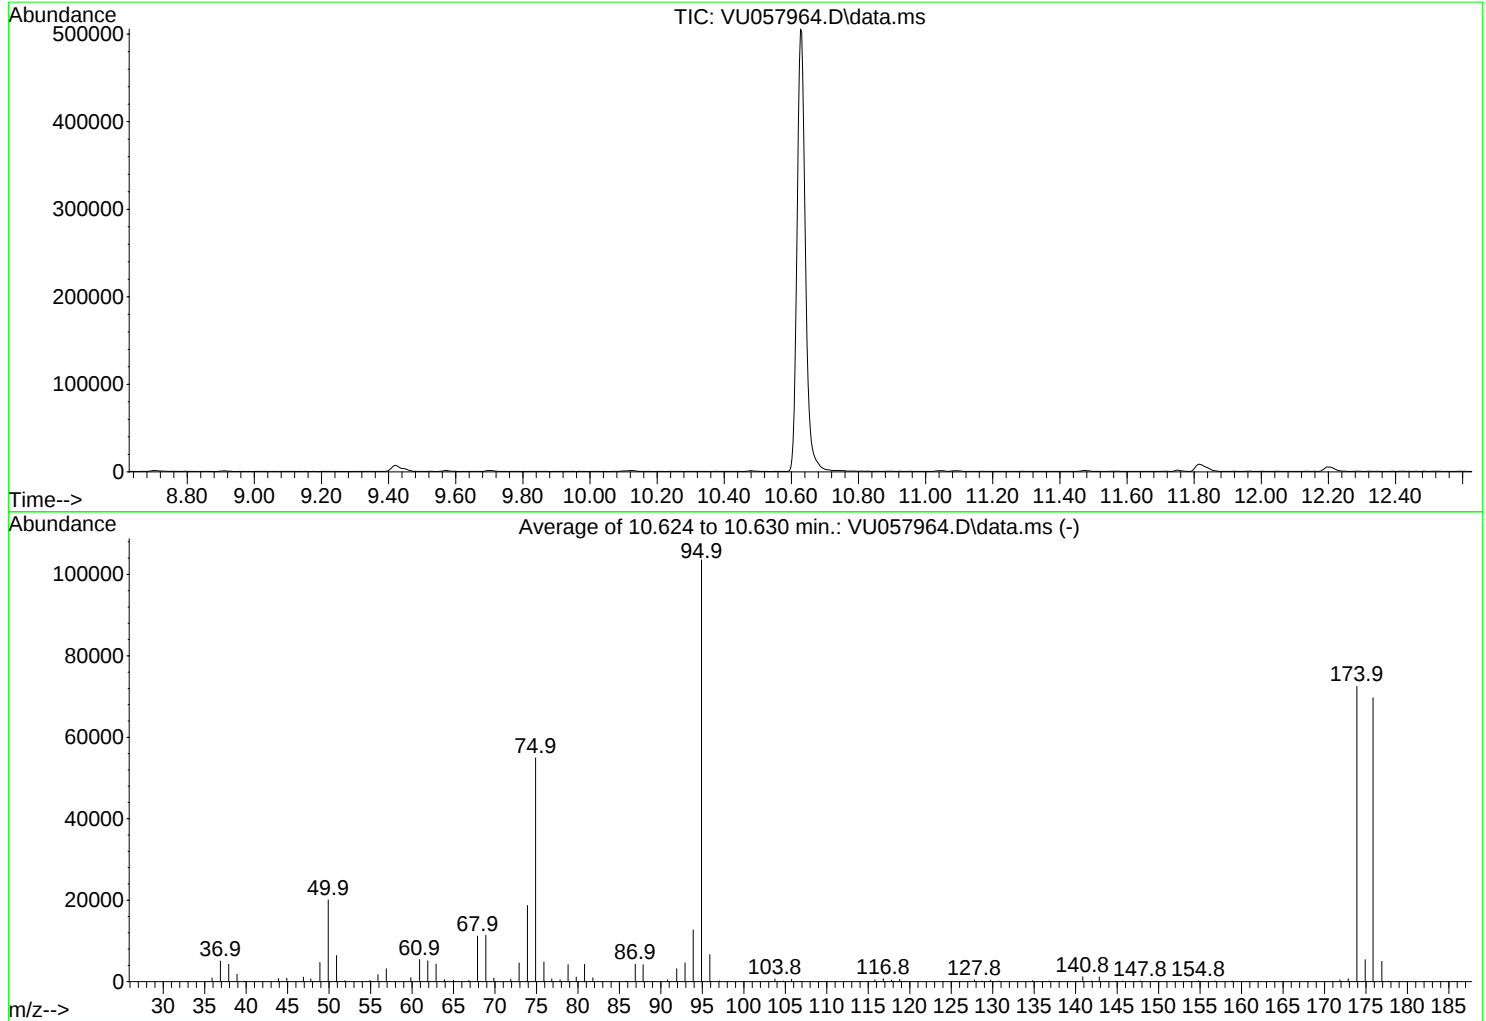

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.4	20061	PASS
75	95	30	80	53.0	54949	PASS
95	95	100	100	100.0	103584	PASS
96	95	5	9	6.4	6630	PASS
173	174	0.00	2	1.0	714	PASS
174	95	50	120	70.0	72504	PASS
175	174	5	9	7.4	5374	PASS
176	174	95	101	96.1	69691	PASS
177	176	5	9	7.2	4998	PASS

m/z	Abundance
39.80	253.0
43.90	239.0

Instrument :
MSVOA_U
ClientSampleId :
BFB115

m/z	Abundance
35.90	879.0
36.90	4993.0
37.90	4046.0
38.90	1722.0
39.80	333.0
43.90	902.0
44.90	819.0
46.90	1056.0
47.80	636.0
48.90	4676.0
49.90	19544.0
50.90	6316.0
51.90	244.0
54.90	286.0
55.90	1634.0
56.90	3033.0
57.90	166.0
59.80	924.0
60.90	5255.0
61.90	4906.0
62.90	4173.0
63.90	439.0
65.00	366.0
66.80	305.0
67.90	10447.0
68.90	10872.0
69.80	896.0
71.90	520.0
72.90	4373.0
73.90	17856.0
74.90	52976.0
75.90	4899.0
76.80	619.0
77.90	434.0
78.80	3930.0
79.80	1067.0
80.80	3902.0
81.80	800.0
85.80	136.0
86.90	4158.0
87.80	3781.0
90.80	407.0
91.90	3047.0
92.90	4466.0
93.90	12016.0
94.90	98696.0
95.90	6501.0
97.00	235.0
103.70	603.0
104.80	155.0
105.70	522.0
106.80	100.0
109.80	109.0
110.60	116.0
115.80	440.0
116.80	691.0
117.80	334.0
118.80	594.0
127.80	392.0
128.70	167.0
129.70	372.0
130.70	117.0
134.80	211.0
136.80	155.0
140.90	1067.0
141.90	117.0
142.90	1125.0
143.70	125.0
145.70	133.0
147.80	207.0
149.70	103.0
154.80	201.0
156.80	134.0
158.90	125.0
171.80	380.0
172.90	728.0
173.90	67024.0
174.90	5029.0
175.90	65304.0
176.90	4766.0
177.80	108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB115

m/z	Abundance
35.90	955.0
36.90	5211.0
37.90	4343.0
38.90	1869.0
39.80	366.0
43.90	1024.0
44.90	886.0
45.90	107.0
46.90	1136.0
47.80	679.0
48.90	4894.0
49.90	20496.0
50.90	6586.0
51.90	249.0
54.90	304.0
55.90	1763.0
56.90	3295.0
57.90	123.0
59.90	1000.0
60.90	5581.0
61.90	5219.0
62.90	4448.0
63.90	504.0
65.00	366.0
66.90	307.0
67.90	11465.0
68.90	11849.0
69.90	978.0
71.90	579.0
72.90	4717.0
73.90	19248.0
74.90	56408.0
75.90	4888.0
76.80	693.0
77.80	479.0
78.80	4209.0
79.80	1188.0
80.80	4338.0
81.80	980.0
85.80	147.0
86.90	4418.0
87.90	4235.0
90.80	441.0
91.90	3291.0
92.90	4781.0
93.90	12974.0
94.90	106760.0
95.90	6828.0
97.10	219.0
103.70	687.0
104.70	151.0
105.80	607.0
109.80	101.0
110.60	125.0
110.90	127.0
115.80	504.0
116.80	773.0
117.80	420.0
118.80	616.0
127.80	448.0
128.70	177.0
129.70	355.0
130.80	146.0
134.80	256.0
136.80	143.0
140.90	1274.0
141.90	161.0
142.80	1184.0
144.90	135.0
145.70	150.0
147.80	223.0
149.70	124.0
153.80	109.0
154.80	254.0
156.80	221.0
158.80	145.0
171.80	420.0
172.90	739.0
173.90	74720.0
174.90	5528.0
175.80	71680.0
176.90	5222.0
177.70	107.0

Instrument :
MSVOA_U
ClientSampleId :
BFB115

m/z	Abundance
35.90	879.0
36.90	4973.0
37.90	4356.0
38.90	1865.0
39.80	360.0
43.90	1033.0
44.90	879.0
46.90	1127.0
47.80	675.0
48.90	4530.0
49.90	20144.0
50.90	6331.0
51.90	210.0
54.90	270.0
55.90	1766.0
56.90	3204.0
59.90	1071.0
60.90	5391.0
61.90	5157.0
62.90	4338.0
63.90	458.0
65.00	299.0
66.90	299.0
67.90	11623.0
68.90	11642.0
69.90	881.0
71.90	564.0
72.90	4756.0
73.90	19040.0
74.90	55464.0
75.90	4726.0
76.90	712.0
77.80	493.0
78.80	4326.0
79.80	1183.0
80.80	4520.0
81.80	1052.0
82.80	110.0
85.80	144.0
86.90	4279.0
87.90	4458.0
90.80	447.0
91.90	3235.0
92.90	4600.0
93.90	13069.0
94.90	105296.0
95.90	6561.0
97.10	177.0
103.80	725.0
104.80	142.0
105.80	618.0
110.90	140.0
115.80	481.0
116.80	741.0
117.80	472.0
118.80	609.0
127.80	426.0
128.70	154.0
129.80	371.0
130.80	159.0
134.80	253.0
136.80	130.0
140.80	1360.0
141.90	171.0
142.80	1198.0
144.80	145.0
145.70	160.0
147.80	206.0
149.70	113.0
154.80	250.0
156.80	262.0
158.80	170.0
160.80	101.0
171.90	459.0
172.80	675.0
173.90	75768.0
174.90	5565.0
175.80	72088.0
176.90	5007.0
177.70	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB115