

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU030119\
 Data File : VU029756.D
 Acq On : 01 Mar 2019 12:09
 Operator : JC/SP
 Sample : K1660-13
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CWK13

Quant Time: Mar 04 11:43:02 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR022119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Mar 01 22:12:01 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	236909	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	233248	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	117810	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	59747	3.86	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.20%
7) Chloroethane-d5	1.68	69	64548	4.43	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.60%
11) 1,1-Dichloroethene-d2	2.27	63	95125	2.86	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.20%#
20) 2-Butanone-d5	4.19	46	228556	65.34	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	130.68%#
24) Chloroform-d	4.65	84	131895	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.80%
26) 1,2-Dichloroethane-d4	5.31	65	78386	5.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.40%
32) Benzene-d6	5.34	84	293892	4.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.20%
36) 1,2-Dichloropropane-d6	6.33	67	95509	5.48	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	109.60%
41) Toluene-d8	7.56	98	256337	4.37	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.40%
43) trans-1,3-Dichloropropene-	7.85	79	33956	4.75	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.00%
46) 2-Hexanone-d5	8.31	63	212552	60.63	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	121.26%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	87746	5.61	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	112.20%
64) 1,2-Dichlorobenzene-d4	11.86	152	114851	4.96	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.20%


Target Compounds					Ovalue
13) Acetone	2.32	43	11851	4.716 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU030119\
Data File : VU029756.D
Acq On : 01 Mar 2019 12:09
Operator : JC/SP
Sample : K1660-13
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CWK13

Quant Time: Mar 04 11:43:02 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR022119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Mar 01 22:12:01 2019
Response via : Initial Calibration

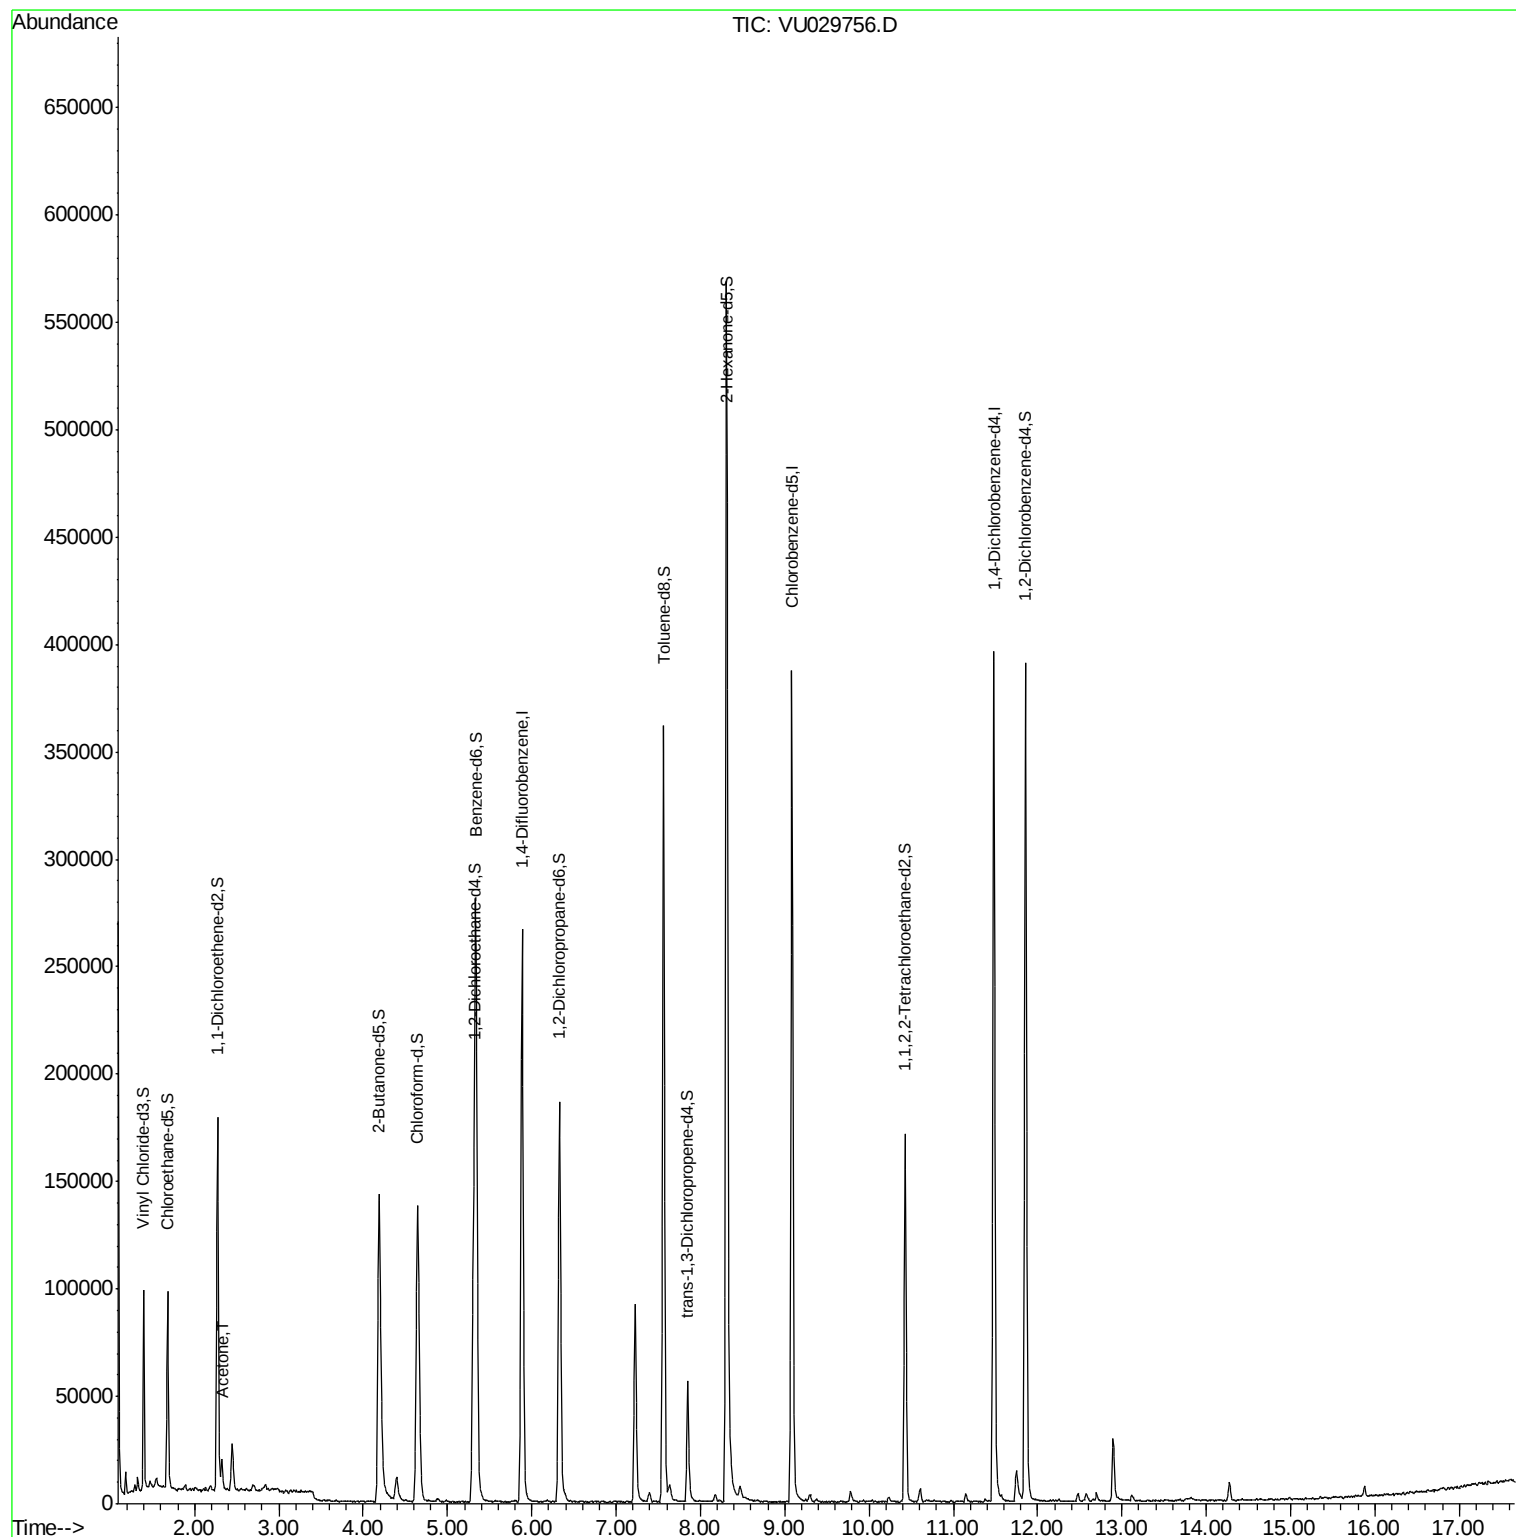

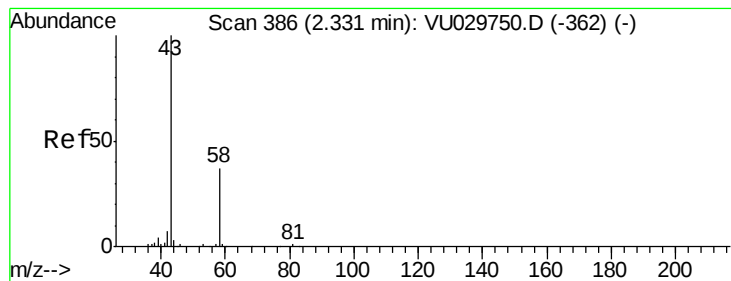

#13

Acetone

Concen: 4.716 ug/L

RT: 2.32 min Scan# 383

Delta R.T. -0.01 min

Lab File: VU029756.D

Acq: 01 Mar 2019 12:09

Instrument :

MSVOA_U

ClientSampleId :

CWK13

Tot Ion: 43 Resp: 11851

Ion Ratio Lower Upper

43 100

58 39.2 0.0 70.2

