

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU030119\
 Data File : VU029759.D
 Acq On : 01 Mar 2019 13:20
 Operator : JC/SP
 Sample : K1660-13RE
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CWK13RE

Quant Time: Mar 01 23:01:03 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR022119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Mar 01 22:12:01 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	236249	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	228514	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	114357	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	91157	5.91	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	118.20%
7) Chloroethane-d5	1.68	69	71926	4.96	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.20%
11) 1,1-Dichloroethene-d2	2.27	63	127870	3.86	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.20%
20) 2-Butanone-d5	4.19	46	181320	51.98	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.96%
24) Chloroform-d	4.65	84	130516	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.00%
26) 1,2-Dichloroethane-d4	5.31	65	72679	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.00%
32) Benzene-d6	5.34	84	312123	5.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.40%
36) 1,2-Dichloropropane-d6	6.33	67	94173	5.52	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	110.40%
41) Toluene-d8	7.56	98	287666	5.01	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.20%
43) trans-1,3-Dichloropropene-	7.85	79	33561	4.79	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.80%
46) 2-Hexanone-d5	8.31	63	171718	50.00	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.00%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	73817	4.81	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.20%
64) 1,2-Dichlorobenzene-d4	11.86	152	114879	5.11	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.20%


Target Compounds				Ovalue
13) Acetone	2.32	43	11601	4.629 ug/L 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU030119\
Data File : VU029759.D
Acq On : 01 Mar 2019 13:20
Operator : JC/SP
Sample : K1660-13RE
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CWK13RE

Quant Time: Mar 01 23:01:03 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR022119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Mar 01 22:12:01 2019
Response via : Initial Calibration

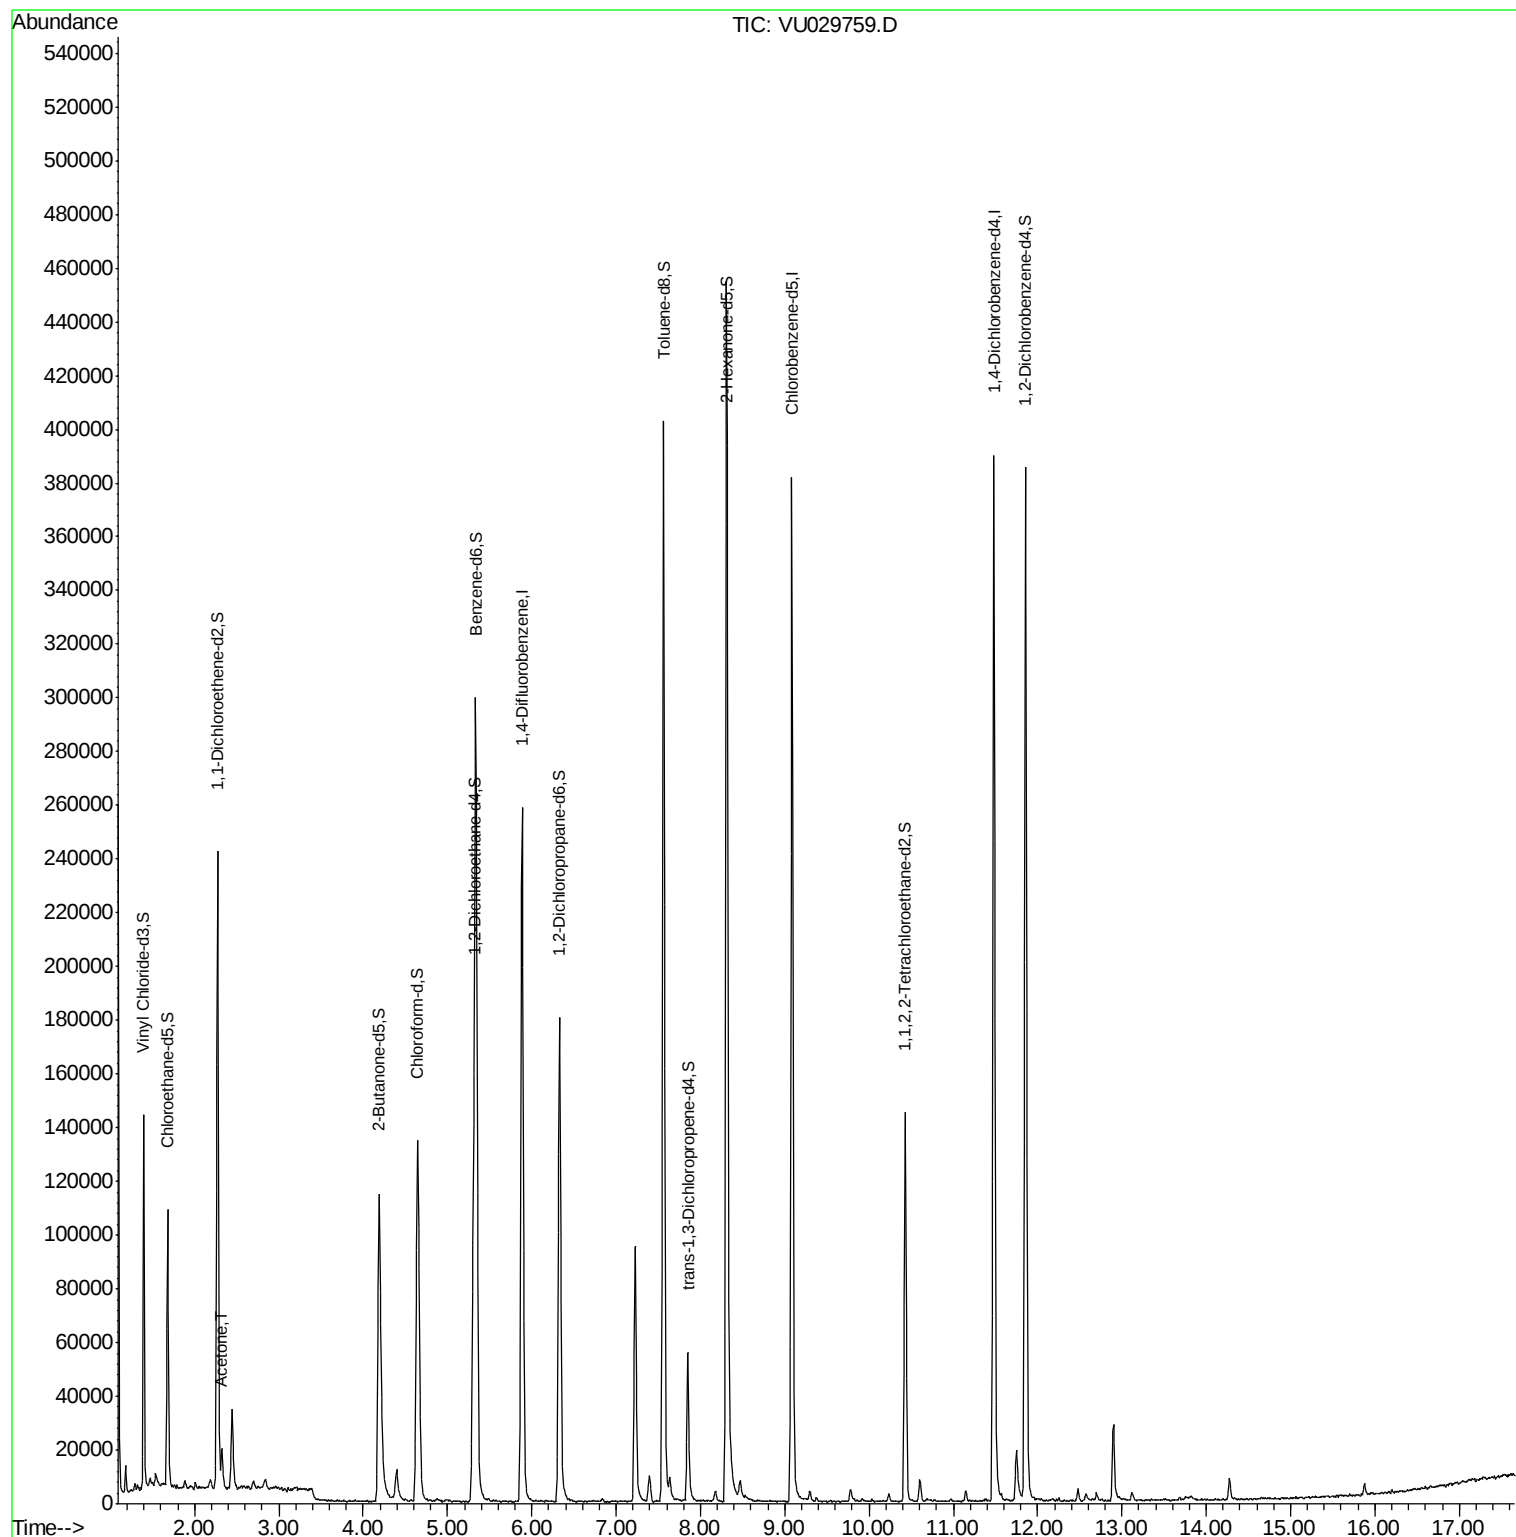

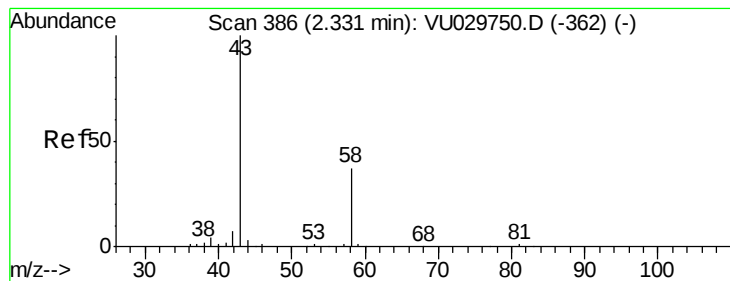

#13

Acetone

Concen: 4.629 ug/L

RT: 2.32 min Scan# 383

Delta R.T. -0.01 min

Lab File: VU029759.D

Acq: 01 Mar 2019 13:20


Instrument :
MSVOA_U
ClientSampleId :
CWK13RE

Tot Ion: 43 Resp: 11601

Ion Ratio Lower Upper

43 100

58 37.6 0.0 70.2

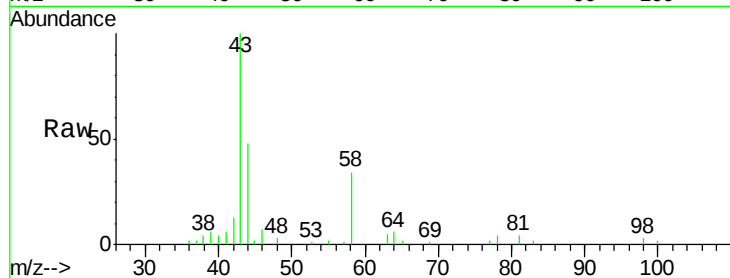

Abundance Ion 43.05 (42.75 to 43.75): VU0

Ion 58.05 (57.75 to 58.75): VU0

