

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU030119\
 Data File : VU029760.D
 Acq On : 01 Mar 2019 13:44
 Operator : JC/SP
 Sample : K1660-12RE
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CWK10RE

Quant Time: Mar 04 11:43:45 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR022119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Mar 01 22:12:01 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	237293	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	228893	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	114644	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	87503	5.65	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	113.00%
7) Chloroethane-d5	1.68	69	69060	4.74	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.80%
11) 1,1-Dichloroethene-d2	2.27	63	120933	3.63	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.60%
20) 2-Butanone-d5	4.19	46	172093	49.12	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.24%
24) Chloroform-d	4.65	84	122236	4.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.60%
26) 1,2-Dichloroethane-d4	5.31	65	69924	4.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.80%
32) Benzene-d6	5.34	84	300981	5.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.40%
36) 1,2-Dichloropropane-d6	6.33	67	89507	5.24	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.80%
41) Toluene-d8	7.56	98	276072	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.00%
43) trans-1,3-Dichloropropene-	7.85	79	31893	4.54	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.80%
46) 2-Hexanone-d5	8.31	63	165286	48.05	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.10%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	71419	4.65	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.00%
64) 1,2-Dichlorobenzene-d4	11.86	152	110774	4.91	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.20%


Target Compounds					Ovalue
13) Acetone	2.32	43	10993	4.367 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU030119\
Data File : VU029760.D
Acq On : 01 Mar 2019 13:44
Operator : JC/SP
Sample : K1660-12RE
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CWK10RE

Quant Time: Mar 04 11:43:45 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR022119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Mar 01 22:12:01 2019
Response via : Initial Calibration

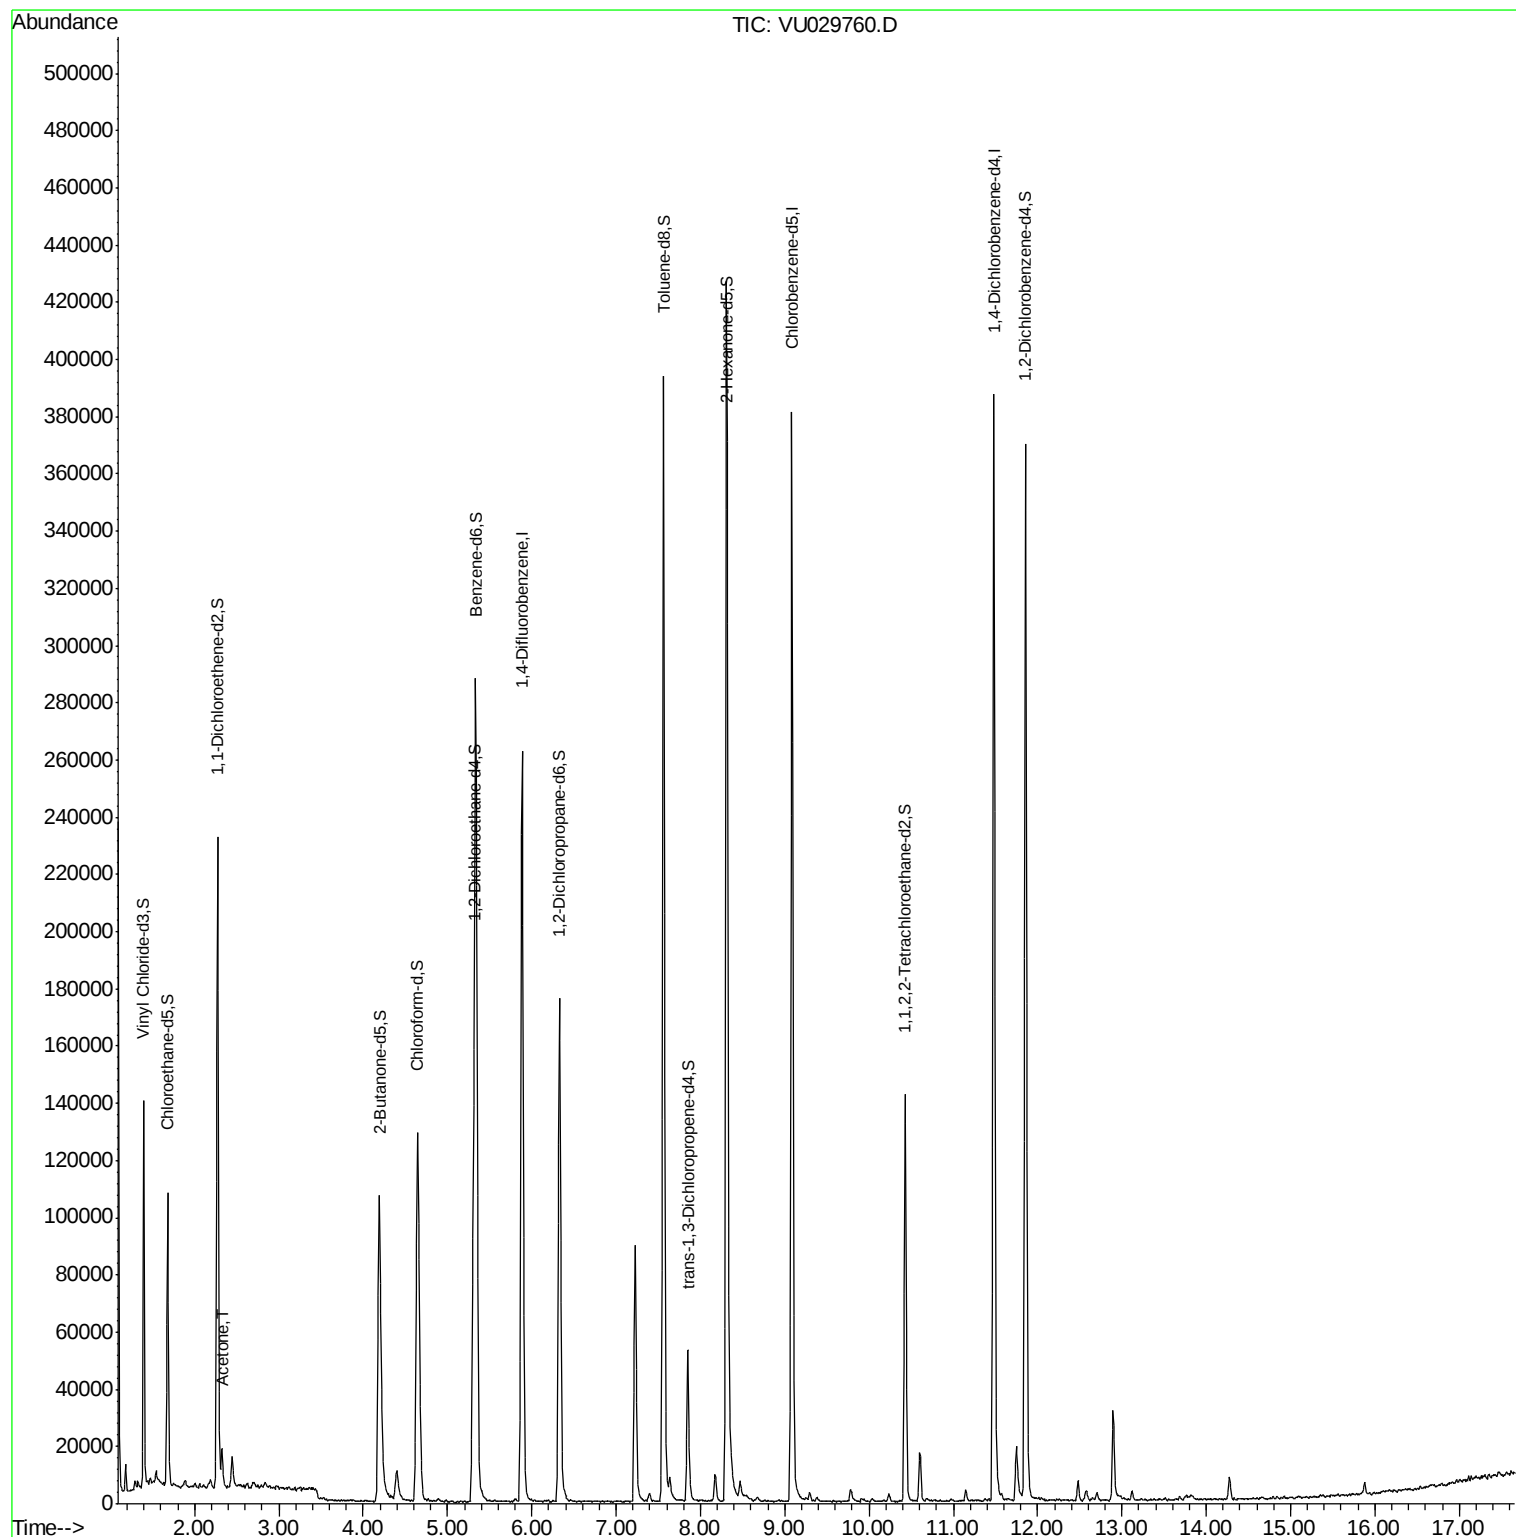

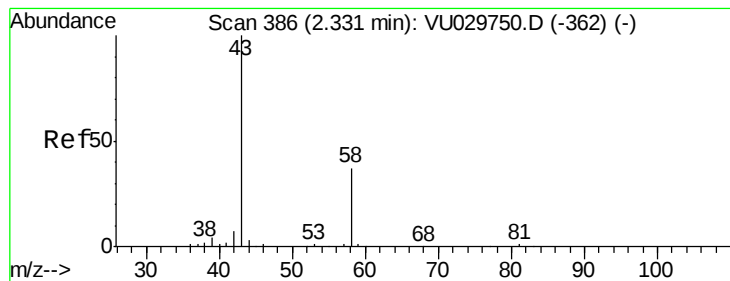

#13

Acetone

Concen: 4.367 ug/L

RT: 2.32 min Scan# 383

Delta R.T. -0.01 min

Lab File: VU029760.D

Acq: 01 Mar 2019 13:44

Instrument :
MSVOA_U
ClientSampleId :
CWK10RE

Tot Ion: 43 Resp: 10993

Ion Ratio Lower Upper

43 100

58 35.5 0.0 70.2

