


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030119\
Data File : VU029749.D
Acq On : 01 Mar 2019 08:20
Operator : JC/SP
Sample : BFB53
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB53

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR022119WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Mar 01 22:12:01 2019

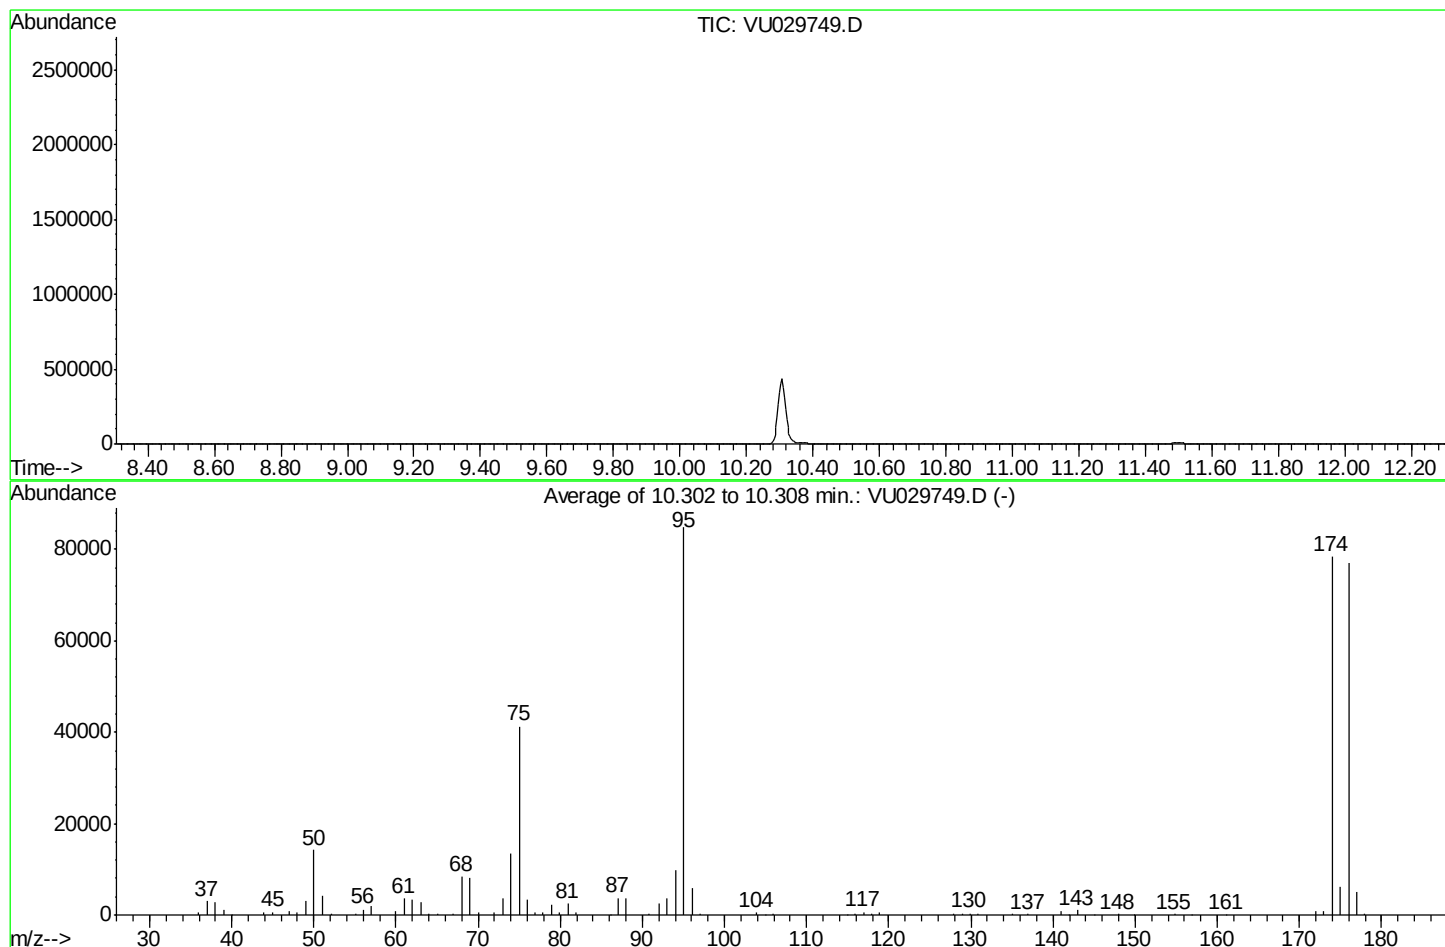

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	14263	PASS
75	95	30	80	48.7	41328	PASS
95	95	100	100	100.0	84853	PASS
96	95	5	9	7.1	6033	PASS
173	174	0.00	2	1.0	805	PASS
174	95	50	120	92.3	78352	PASS
175	174	5	9	8.0	6304	PASS
176	174	95	101	98.5	77157	PASS
177	176	5	9	6.4	4967	PASS

m/z	Abundance
35.90	578.0
37.00	2993.0
38.00	2941.0
39.00	1187.0
40.00	180.0
43.90	982.0
45.00	715.0
47.00	748.0
48.00	408.0
49.00	2935.0
50.00	13861.0
51.00	3967.0
52.10	257.0
55.00	224.0
56.00	1029.0
57.00	1890.0
60.00	816.0
61.00	3459.0
62.00	3398.0
63.10	2927.0
63.90	454.0
65.00	312.0
67.00	261.0
68.00	8051.0
69.00	7628.0
70.00	613.0
71.90	468.0
73.00	3702.0
74.00	13457.0
75.00	39784.0
76.00	3470.0
77.00	515.0
77.80	428.0
78.90	2373.0
80.00	712.0
80.90	2432.0
81.90	471.0
87.00	3761.0
88.00	3434.0
90.80	209.0
92.00	2192.0
93.00	3446.0
94.00	9188.0
95.10	81704.0
96.00	5894.0
97.10	181.0
103.90	373.0
105.90	366.0
114.90	112.0
115.80	259.0
116.90	613.0
117.90	368.0
118.90	510.0
127.90	290.0
128.90	148.0
129.90	352.0
130.90	174.0
135.10	190.0
137.00	124.0
140.90	780.0
141.90	169.0
142.90	1036.0
145.00	112.0
147.90	160.0
154.90	136.0
156.80	131.0
172.00	742.0
173.00	701.0
174.00	73880.0
175.00	5926.0
176.00	72648.0
177.00	4775.0
177.90	150.0
207.10	121.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53

m/z	Abundance
36.00	638.0
37.00	3033.0
38.00	2957.0
39.10	1184.0
40.00	208.0
43.90	924.0
45.00	685.0
47.10	770.0
48.00	449.0
49.00	3108.0
50.00	14824.0
51.00	4187.0
52.10	211.0
55.10	183.0
56.00	1238.0
57.00	1921.0
60.00	845.0
61.00	3637.0
62.00	3590.0
63.00	2994.0
64.00	387.0
65.00	374.0
67.00	274.0
68.00	8576.0
69.00	8239.0
70.00	621.0
71.90	528.0
73.00	3637.0
74.00	14087.0
75.00	42832.0
76.00	3484.0
77.00	515.0
77.80	479.0
78.90	2476.0
79.90	729.0
80.90	2638.0
81.90	525.0
86.20	171.0
87.00	3792.0
88.00	3784.0
90.80	272.0
92.00	2515.0
93.00	3694.0
94.00	10077.0
95.00	87360.0
96.00	6290.0
97.10	156.0
103.90	465.0
105.00	118.0
105.90	441.0
114.90	115.0
115.90	275.0
116.90	659.0
117.90	374.0
118.90	619.0
127.90	268.0
129.00	176.0
129.90	411.0
130.80	170.0
135.00	159.0
137.00	175.0
141.00	810.0
141.90	159.0
142.90	1025.0
148.00	168.0
154.80	209.0
156.90	137.0
161.10	109.0
172.00	814.0
173.00	839.0
174.00	81056.0
175.00	6557.0
176.00	79824.0
177.00	5057.0
177.90	179.0
207.10	128.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53

m/z	Abundance
36.00	626.0
37.00	2957.0
38.00	2858.0
39.10	1168.0
40.00	224.0
43.90	850.0
45.00	592.0
47.00	813.0
48.00	441.0
49.00	3060.0
50.00	14104.0
51.00	4081.0
52.10	139.0
55.10	140.0
56.00	1268.0
57.00	1887.0
59.90	776.0
61.00	3545.0
62.00	3421.0
63.00	2765.0
64.10	346.0
65.00	442.0
66.90	206.0
68.00	8286.0
69.00	8140.0
70.00	536.0
72.00	516.0
73.00	3432.0
74.00	13246.0
75.00	41368.0
76.00	3271.0
76.90	417.0
77.80	408.0
79.00	2289.0
79.90	690.0
80.90	2488.0
81.90	565.0
86.10	156.0
87.00	3461.0
88.00	3745.0
90.80	272.0
92.00	2592.0
93.00	3556.0
94.00	9906.0
95.00	85496.0
96.10	5916.0
97.00	145.0
103.90	484.0
105.00	142.0
105.90	472.0
116.00	284.0
116.90	643.0
117.90	311.0
118.90	637.0
127.90	252.0
128.90	185.0
129.90	360.0
130.80	131.0
134.90	124.0
137.00	210.0
141.00	836.0
141.80	121.0
143.00	956.0
148.00	168.0
149.80	113.0
154.80	284.0
157.00	148.0
171.90	781.0
173.00	875.0
174.00	80120.0
175.00	6431.0
176.00	79000.0
177.00	5071.0
177.90	204.0
207.00	164.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53

m/z	Abundance
39.80	166.0
43.90	432.0
207.00	153.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53