
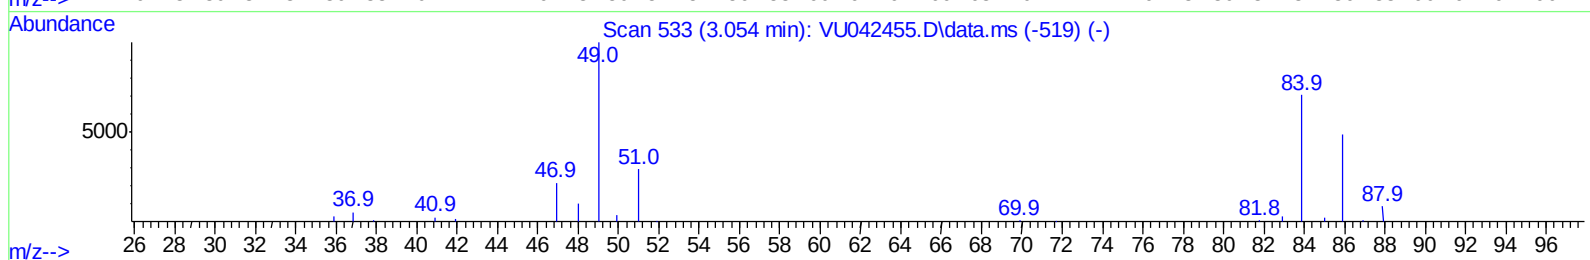
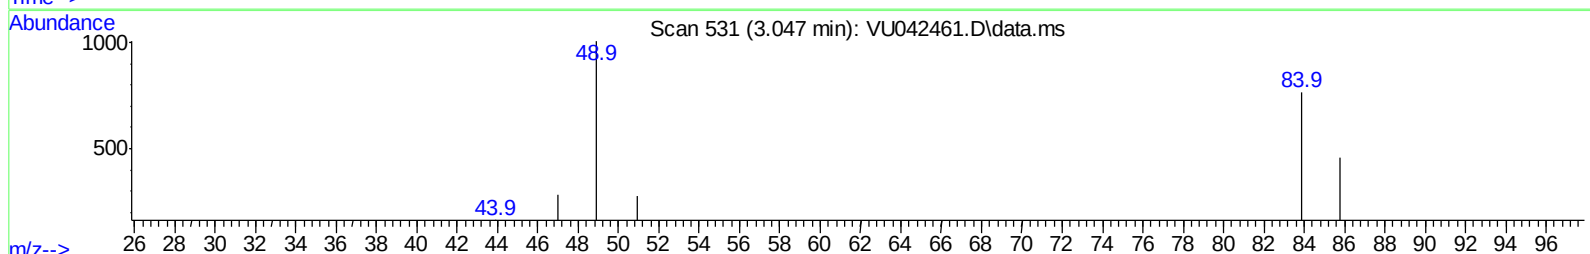


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030121\
 Data File : VU042461.D
 Acq On : 01 Mar 2021 13:12
 Operator : SY/MD
 Sample : VU0301WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Quant Time: Mar 02 14:47:15 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030121WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Mar 02 14:41:09 2021
 Response via : Initial Calibration

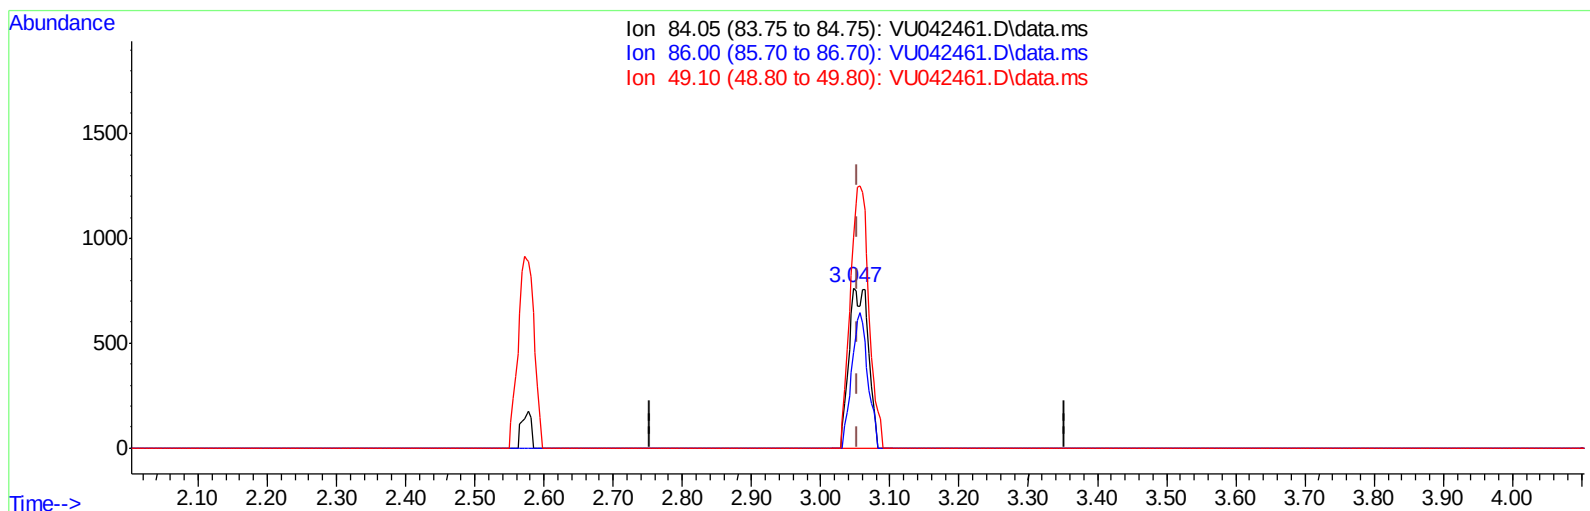

TIC: VU042461.D\data.ms

(16) Methylene chloride (T)**3.047min (-0.006) 0.20 ug/L m****response 1509**

Ion	Exp%	Act%
84.05	100.00	100.00
86.00	69.50	60.16
49.10	141.90	131.98
0.00	0.00	0.00