

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030121\
 Data File : VU042458.D
 Acq On : 01 Mar 2021 11:13
 Operator : SY/MD
 Sample : VIBLK
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Quant Time: Mar 02 14:44:12 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030121WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Mar 02 14:41:09 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.260	114	111588	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.427	117	107729	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.822	152	56715	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	23841	5.04	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.80%
7) Chloroethane-d5	1.919	69	24748	4.99	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.80%
11) 1,1-Dichloroethene-d2	2.575	65	14779	4.90	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	98.00%
20) 2-Butanone-d5	4.649	46	140299	49.70	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.40%
24) Chloroform-d	5.073	84	70949	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.60%
26) 1,2-Dichloroethane-d4	5.713	65	45238	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.80%
32) Benzene-d6	5.736	84	129918	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.60%
36) 1,2-Dichloropropane-d6	6.700	67	43161	4.81	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.20%
41) Toluene-d8	7.906	98	117626	4.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.20%
43) trans-1,3-Dichloroprop...	8.189	79	16889	4.63	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.60%
46) 2-Hexanone-d5	8.649	63	96371	48.20	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.40%
56) 1,1,2,2-Tetrachloroeth...	10.767	84	37407	4.59	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.80%
66) 1,2-Dichlorobenzene-d4	12.201	152	49586	5.03	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.60%
Target Compounds						Qvalue
16) Methylene chloride	3.054	84	1092	0.13	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030121\
Data File : VU042458.D
Acq On : 01 Mar 2021 11:13
Operator : SY/MD
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Time: Mar 02 14:44:12 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030121WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Mar 02 14:41:09 2021
Response via : Initial Calibration

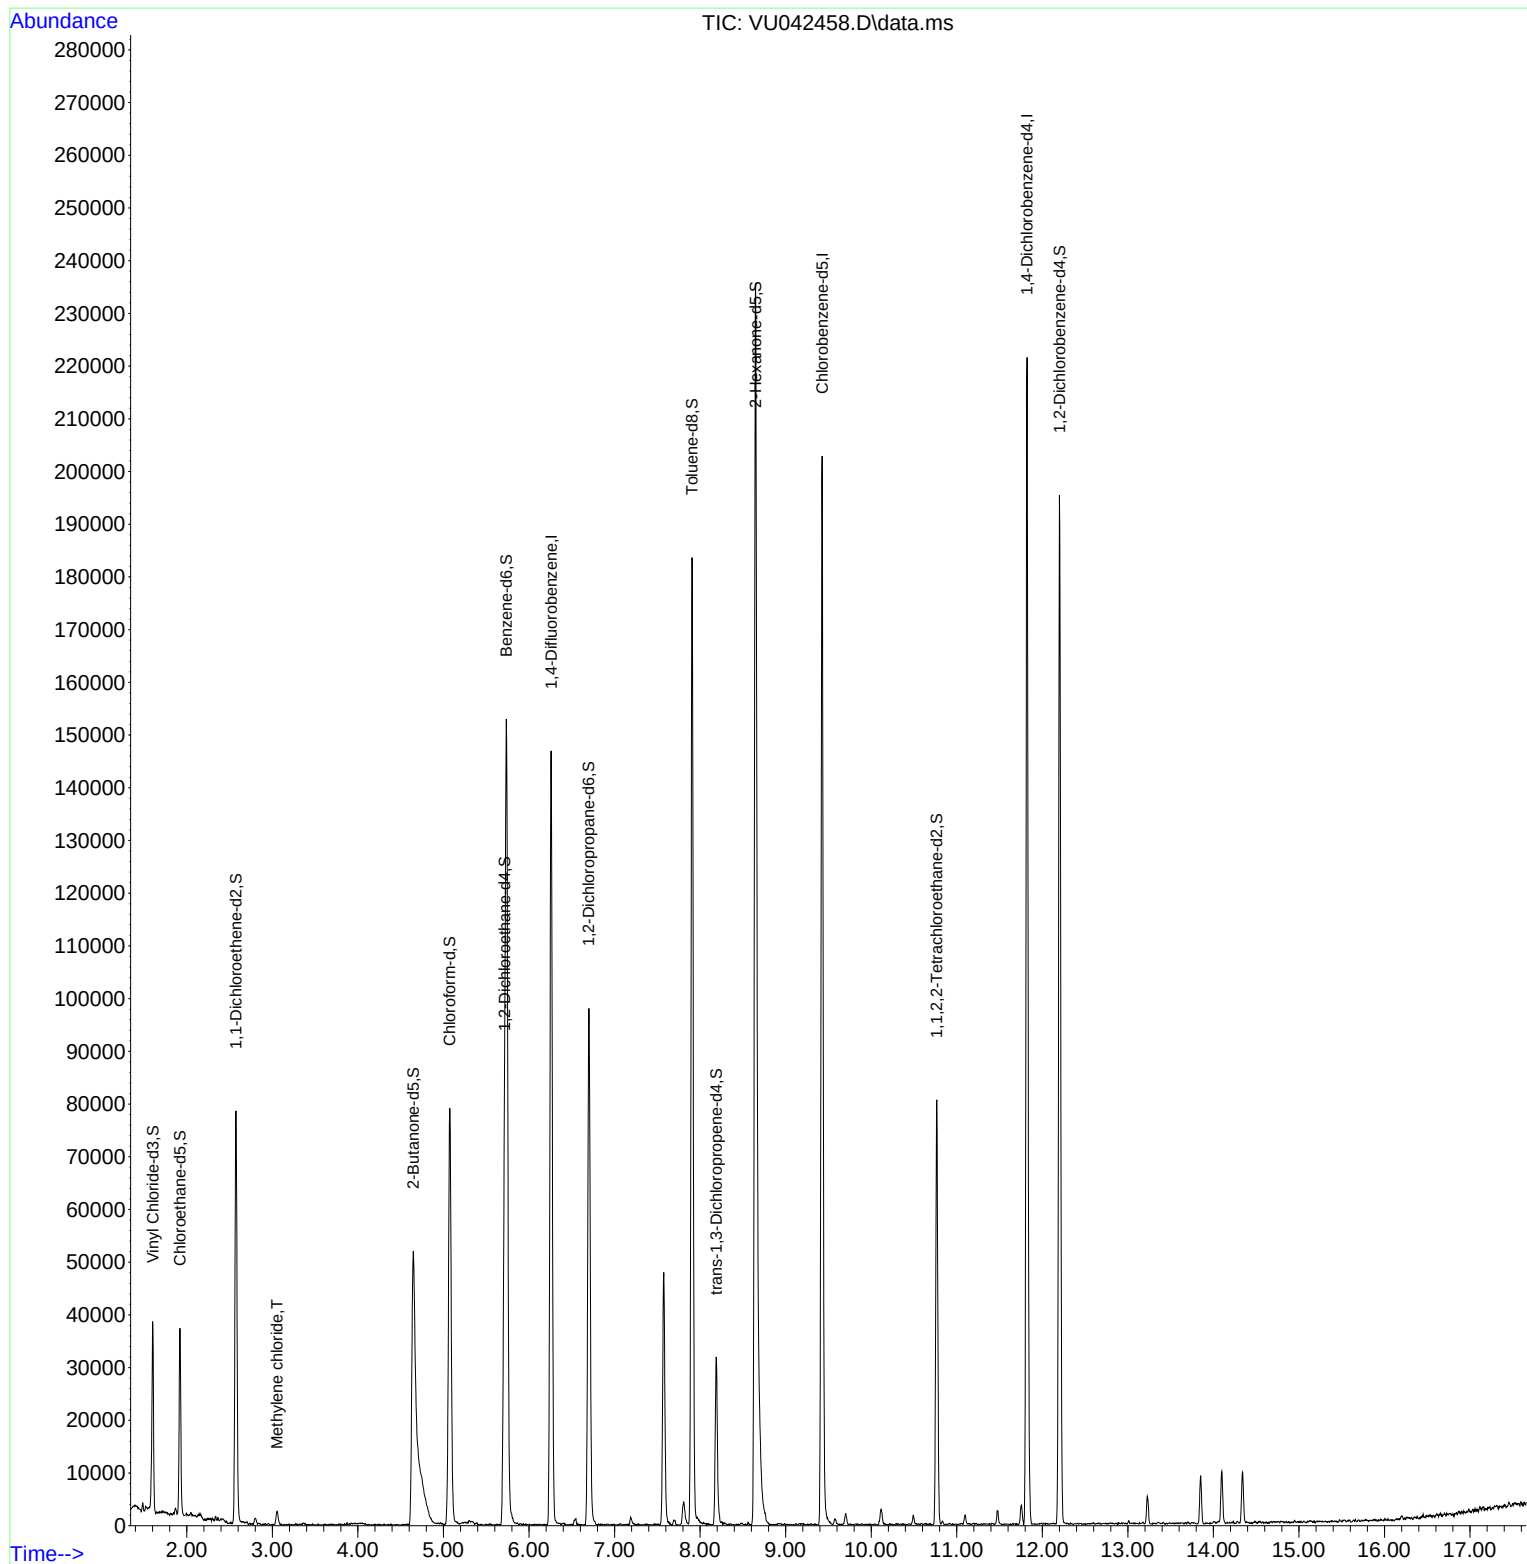

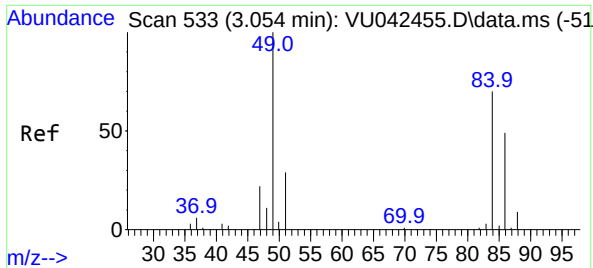

#16
Methylene chloride
Concen: 0.13 ug/L
RT: 3.054 min Scan# 533
Delta R.T. 0.000 min
Lab File: VU042458.D
Acq: 01 Mar 2021 11:13

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Tgt Ion: 84 Resp: 1092

Ion	Ratio	Lower	Upper
84	100		
86	64.6	48.6	90.3
49	141.5	99.3	184.5

