
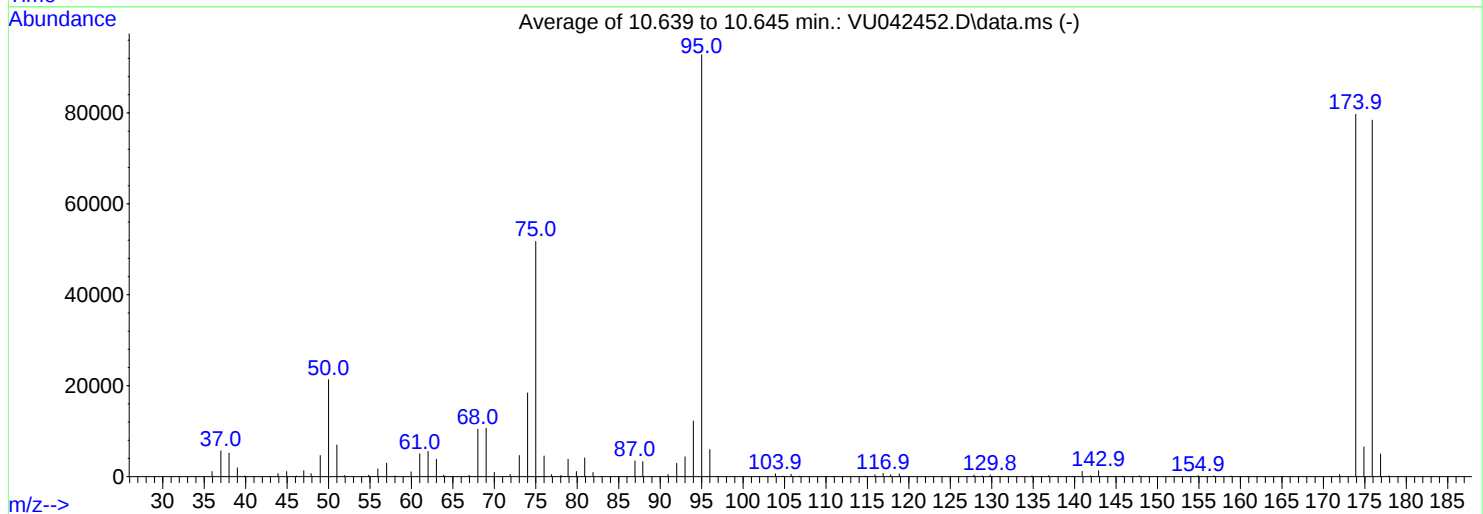


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030121\
Data File : VU042452.D
Acq On : 01 Mar 2021 08:39
Operator : SY/MD
Sample : BFB39
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB390

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030121WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Mar 02 14:41:09 2021

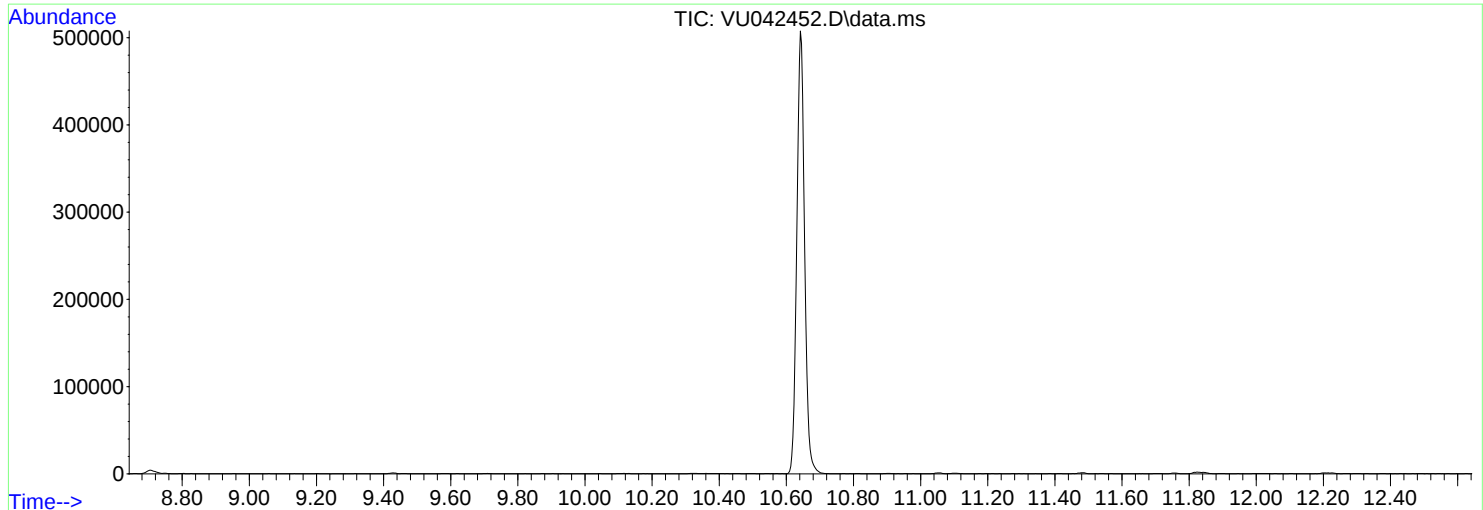

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.0	21323	PASS
75	95	30	80	55.8	51755	PASS
95	95	100	100	100.0	92779	PASS
96	95	5	9	6.4	5935	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.9	79731	PASS
175	174	5	9	8.2	6534	PASS
176	174	95	101	98.4	78416	PASS
177	176	5	9	6.3	4965	PASS

m/z	Abundance
36.00	1098.0
37.00	5763.0
38.00	5019.0
39.00	1895.0
39.90	198.0
43.90	879.0
44.90	1140.0
46.10	132.0
47.00	1312.0
47.90	585.0
49.00	4845.0
50.00	20800.0
51.00	6916.0
51.90	251.0
54.80	294.0
55.90	1741.0
57.00	2871.0
58.00	160.0
59.90	890.0
61.00	5057.0
62.00	5461.0
63.00	3702.0
63.90	345.0
64.80	152.0
67.00	254.0
68.00	10183.0
69.00	10368.0
70.00	925.0
71.90	525.0
73.00	4527.0
74.00	17808.0
75.00	49936.0
76.00	4419.0
76.90	401.0
78.00	283.0
78.90	3735.0
79.90	1060.0
80.90	4017.0
81.90	844.0
82.90	142.0
87.00	3407.0
87.90	3139.0
91.00	431.0
92.00	2823.0
93.00	4348.0
94.00	11755.0
95.00	89408.0
96.00	5831.0
96.90	122.0
103.90	573.0
104.80	165.0
105.80	421.0
106.80	105.0
114.70	118.0
115.90	356.0
116.90	708.0
117.80	397.0
118.80	673.0
127.80	339.0
128.80	132.0
129.80	379.0
130.80	106.0
134.90	187.0
136.90	167.0
139.70	114.0
140.90	1146.0
141.90	197.0
142.90	1155.0
145.80	120.0
147.80	200.0
154.90	233.0
156.80	178.0
158.90	123.0
171.10	107.0
171.90	466.0
173.90	75688.0
174.90	6403.0
175.90	73928.0
176.90	4777.0
177.90	239.0

Instrument :
MSVOA_U
ClientSampleId :
BFB390

m/z	Abundance
35.90	1199.0
37.00	5823.0
38.00	5355.0
39.00	2040.0
39.90	177.0
43.90	853.0
45.00	1148.0
46.10	151.0
47.00	1361.0
47.90	699.0
49.00	4752.0
50.00	22136.0
51.00	7195.0
51.90	269.0
54.90	327.0
55.90	1772.0
57.00	3069.0
58.00	182.0
60.00	1133.0
61.00	5225.0
62.00	5711.0
63.00	3941.0
63.90	345.0
65.00	156.0
66.90	290.0
68.00	10870.0
69.00	11028.0
70.00	983.0
71.90	526.0
73.00	4815.0
74.00	19000.0
75.00	53464.0
76.00	4736.0
76.90	478.0
78.10	299.0
78.90	3982.0
79.90	1167.0
80.90	4308.0
81.90	954.0
82.90	116.0
86.90	3590.0
87.90	3412.0
91.00	464.0
92.00	3079.0
93.00	4466.0
94.00	12629.0
95.00	96080.0
96.00	6057.0
96.90	121.0
103.90	696.0
104.80	146.0
105.80	543.0
106.80	115.0
110.80	110.0
114.80	125.0
115.90	438.0
116.90	694.0
117.80	451.0
118.90	621.0
127.90	378.0
128.90	163.0
129.80	412.0
130.90	124.0
134.80	190.0
136.90	226.0
139.70	124.0
140.90	1188.0
141.90	212.0
142.90	1353.0
143.90	102.0
144.90	140.0
145.80	142.0
147.80	213.0
149.80	106.0
154.90	258.0
156.80	207.0
158.90	132.0
160.90	100.0
172.00	507.0
173.90	82432.0
174.90	6793.0
175.90	80792.0
176.90	5173.0
177.90	222.0

Instrument :
MSVOA_U
ClientSampleId :
BFB390

m/z	Abundance
35.90	1077.0
37.00	5424.0
38.00	5188.0
39.00	1873.0
39.90	180.0
42.90	100.0
43.90	793.0
45.00	1090.0
46.10	139.0
47.00	1263.0
47.90	711.0
49.00	4335.0
50.00	21032.0
51.00	6752.0
51.90	262.0
54.90	317.0
56.00	1589.0
57.00	2953.0
58.00	172.0
60.00	1190.0
61.00	4858.0
62.00	5485.0
63.00	3832.0
63.90	339.0
65.00	195.0
66.90	316.0
68.00	10351.0
69.00	10548.0
70.00	930.0
71.90	473.0
73.00	4597.0
74.00	18424.0
75.00	51864.0
76.00	4479.0
76.90	504.0
78.10	300.0
78.90	3800.0
79.90	1109.0
80.90	4080.0
81.90	976.0
82.90	103.0
86.90	3398.0
87.90	3353.0
90.90	454.0
92.00	2879.0
93.00	4292.0
94.00	12377.0
95.00	92848.0
96.00	5916.0
96.90	116.0
103.90	671.0
104.80	113.0
105.80	603.0
106.80	105.0
110.90	128.0
114.80	146.0
115.90	463.0
116.90	666.0
117.80	475.0
118.90	558.0
127.80	354.0
128.90	204.0
129.80	403.0
130.90	123.0
134.80	190.0
136.80	252.0
139.70	108.0
140.90	1114.0
141.90	182.0
142.90	1385.0
144.90	156.0
145.80	155.0
147.80	192.0
149.80	140.0
154.90	269.0
156.80	224.0
158.80	160.0
160.80	116.0
171.10	139.0
172.00	461.0
173.90	81072.0
174.90	6406.0
175.90	80528.0
176.90	4944.0
177.90	168.0

Instrument :
MSVOA_U
ClientSampleId :
BFB390

m/z	Abundance
43.90	181.0

Instrument :
MSVOA_U
ClientSampleId :
BFB390