

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030124\
 Data File : VU057978.D
 Acq On : 01 Mar 2024 12:15
 Operator : MD/SY
 Sample : VU0301WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK141

Quant Time: Mar 01 22:45:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 01 22:42:28 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	151207	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	140294	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	63006	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	49751	4.573	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	91.400%	
7) Chloroethane-d5	1.907	69	41717	4.665	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	93.400%	
11) 1,1-Dichloroethene-d2	2.560	65	22243	4.725	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	94.400%	
20) 2-Butanone-d5	4.618	46	88707	49.487	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	98.980%	
24) Chloroform-d	5.055	84	94396	4.588	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	91.800%	
26) 1,2-Dichloroethane-d4	5.695	65	46097	4.944	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	98.800%	
32) Benzene-d6	5.721	84	196566	4.808	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	96.200%	
36) 1,2-Dichloropropane-d6	6.682	67	61513	4.949	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	99.000%	
41) Toluene-d8	7.891	98	169693	4.581	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	91.600%	
43) trans-1,3-Dichloroprop...	8.177	79	18766	4.391	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	87.800%	
46) 2-Hexanone-d5	8.627	63	69494	48.428	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	96.860%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84	36416	4.778	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	95.600%	
66) 1,2-Dichlorobenzene-d4	12.187	152	52702	5.079	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	101.600%	
Target Compounds						Qvalue
16) Methylene chloride	3.036	84	2813	0.254	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030124\
Data File : VU057978.D
Acq On : 01 Mar 2024 12:15
Operator : MD/SY
Sample : VU0301WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK141


Quant Time: Mar 01 22:45:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 01 22:42:28 2024
Response via : Initial Calibration

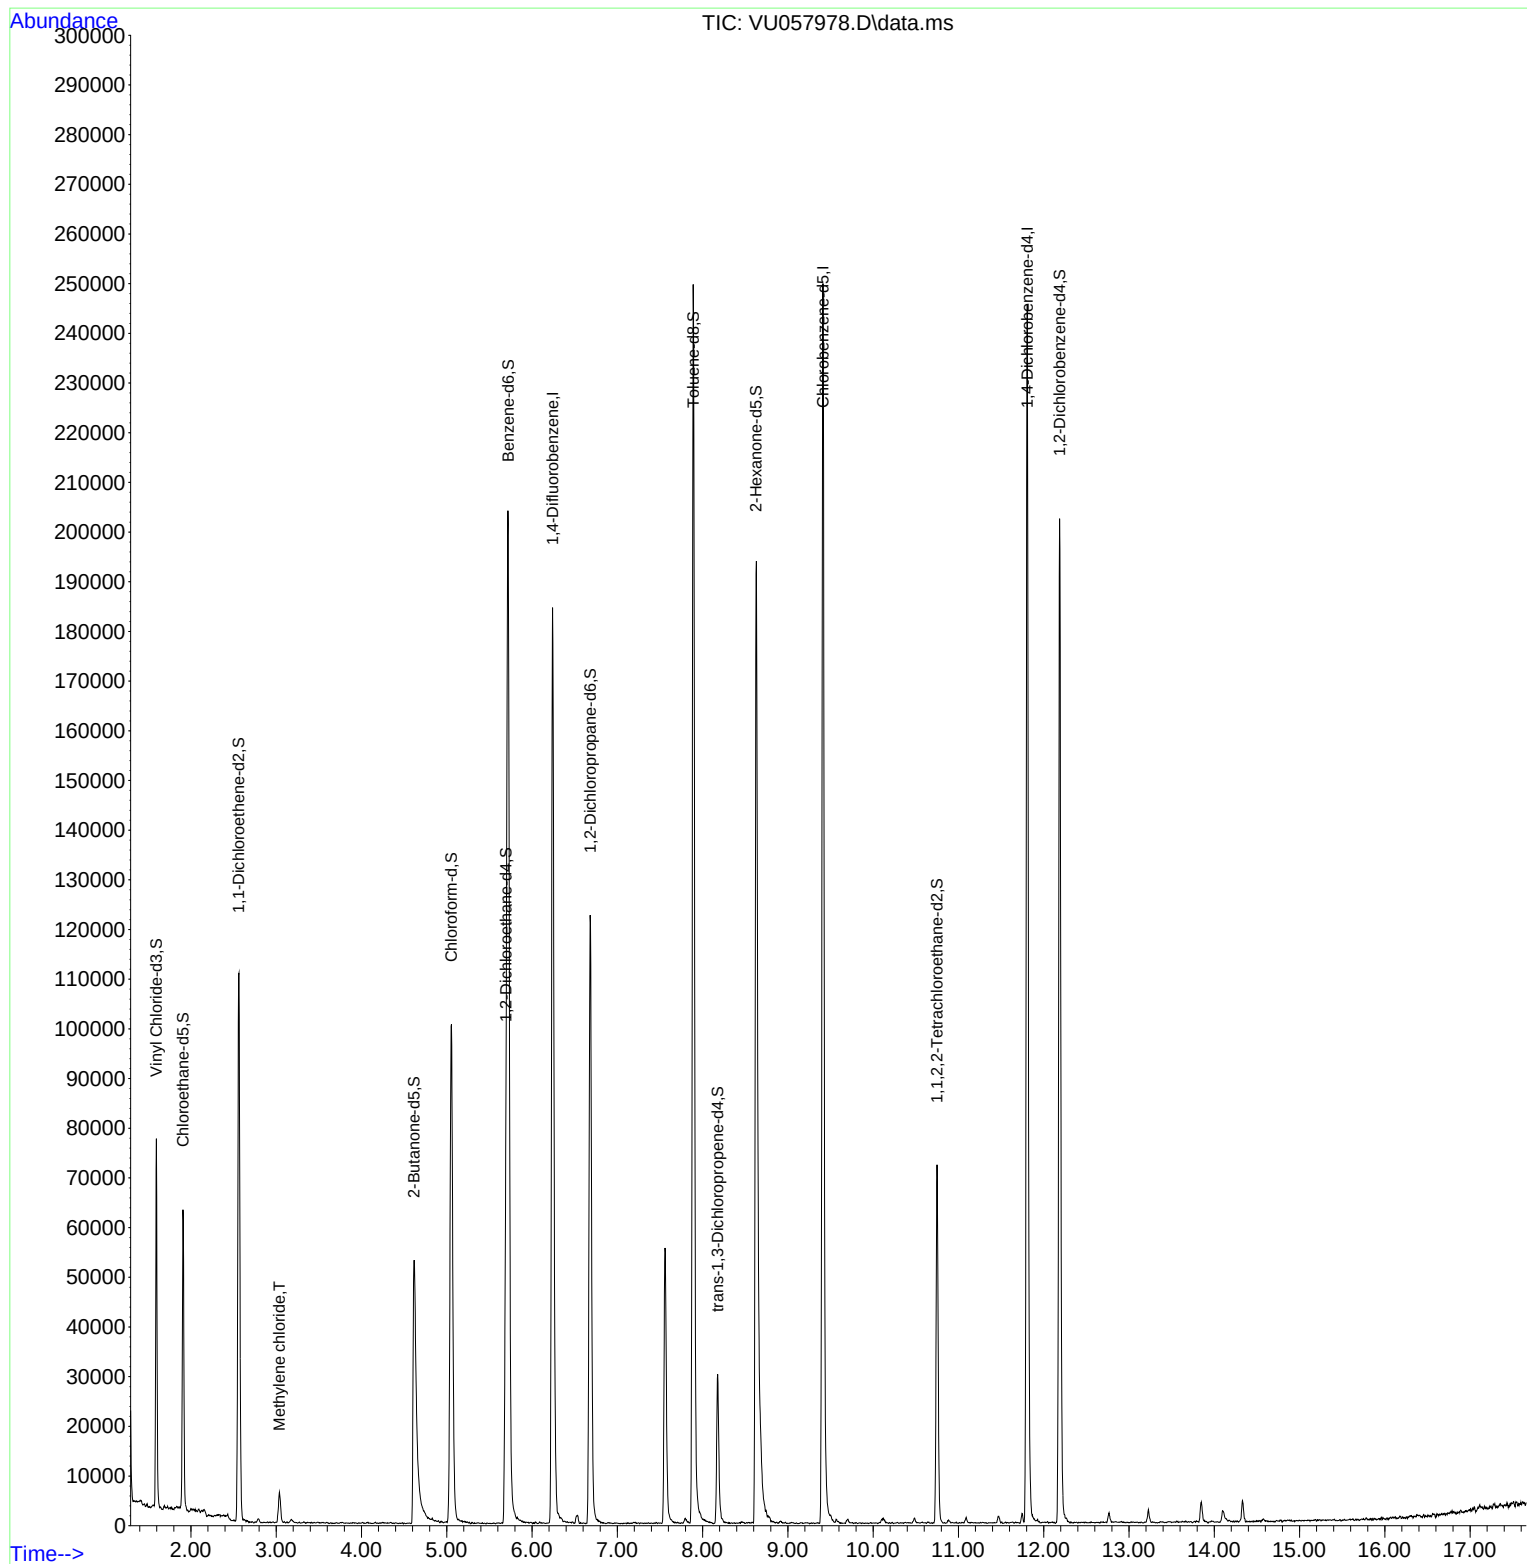

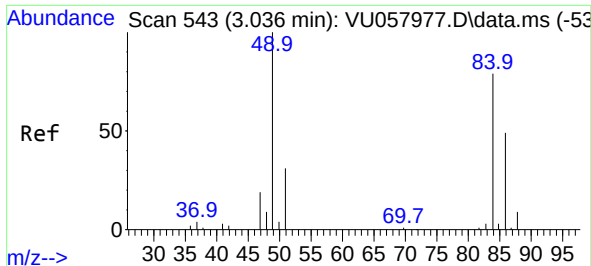

#16
Methylene chloride
Concen: 0.254 ug/L
RT: 3.036 min Scan# 54
Delta R.T. 0.000 min
Lab File: VU057978.D
Acq: 01 Mar 2024 12:15

Instrument :
MSVOA_U
ClientSampleId :
VBLK141

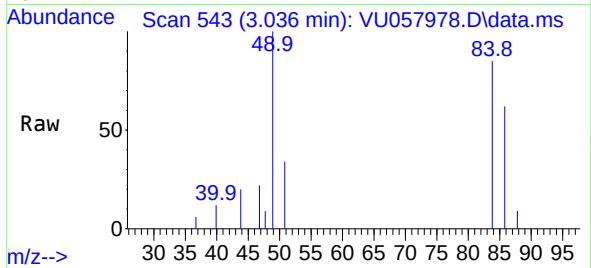

Tgt Ion: 84 Resp: 2813

Ion	Ratio	Lower	Upper
84	100		
86	72.9	44.4	82.4
49	117.8	88.8	165.0

