

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030124\
 Data File : VU057978.D
 Acq On : 01 Mar 2024 12:15
 Operator : MD/SY
 Sample : VU0301WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK141

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU057978.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	108	rVB	74250	80803	15.39%	1.919%
2	1.907	184	192	207	rVB	60575	77288	14.72%	1.835%
3	2.563	384	396	411	rBV	110256	182053	34.67%	4.323%
4	3.039	534	544	558	rVB2	6115	10893	2.07%	0.259%
5	4.618	1023	1035	1084	rBV	53053	156513	29.81%	3.716%
6	5.055	1155	1171	1195	rBV	100246	225540	42.95%	5.356%
7	5.717	1358	1377	1409	rBV3	203830	525101	100.00%	12.469%
8	6.242	1526	1540	1559	rBV	184260	357037	67.99%	8.478%
9	6.682	1665	1677	1700	rBV	122371	244738	46.61%	5.811%
10	7.560	1938	1950	1972	rBV	55465	104260	19.86%	2.476%
11	7.891	2041	2053	2088	rBV	249332	446812	85.09%	10.610%
12	8.177	2131	2142	2157	rBV2	29996	54224	10.33%	1.288%
13	8.631	2272	2283	2316	rBV2	193639	422755	80.51%	10.038%
14	9.412	2512	2526	2552	rBV	249568	438173	83.45%	10.405%
15	10.749	2931	2942	2964	rVB	72127	119488	22.76%	2.837%
16	11.807	3259	3271	3296	rVV	245094	407290	77.56%	9.671%
17	12.187	3378	3389	3411	rBV	202017	338789	64.52%	8.045%
18	13.849	3896	3906	3917	rBV2	4050	6939	1.32%	0.165%
19	14.097	3974	3983	3996	rBV4	2327	5278	1.01%	0.125%
20	14.331	4042	4056	4064	rBV5	4352	7369	1.40%	0.175%




Sum of corrected areas: 4211343

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030124\
Data File : VU057978.D
Acq On : 01 Mar 2024 12:15
Operator : MD/SY
Sample : VU0301WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK141

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

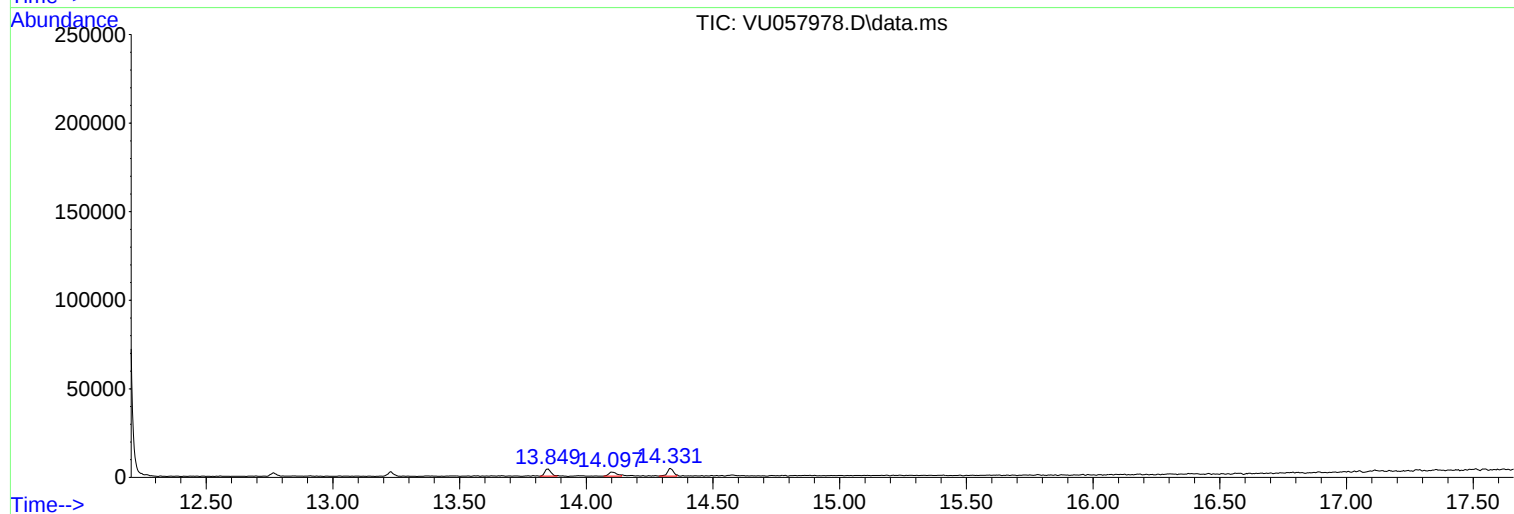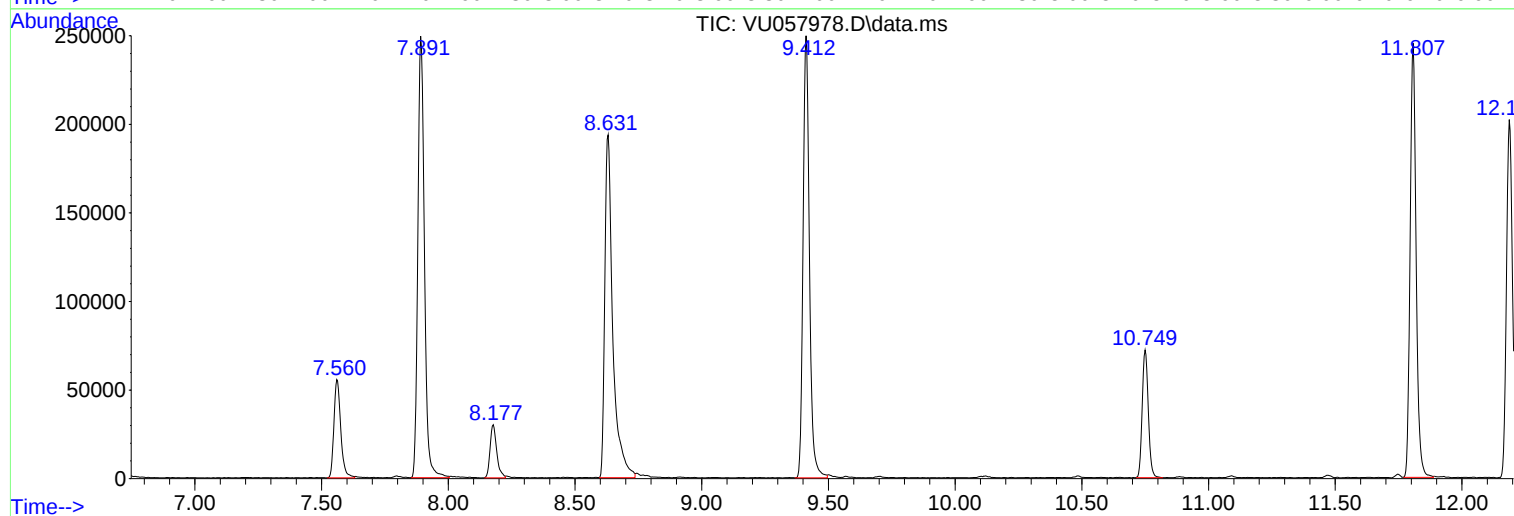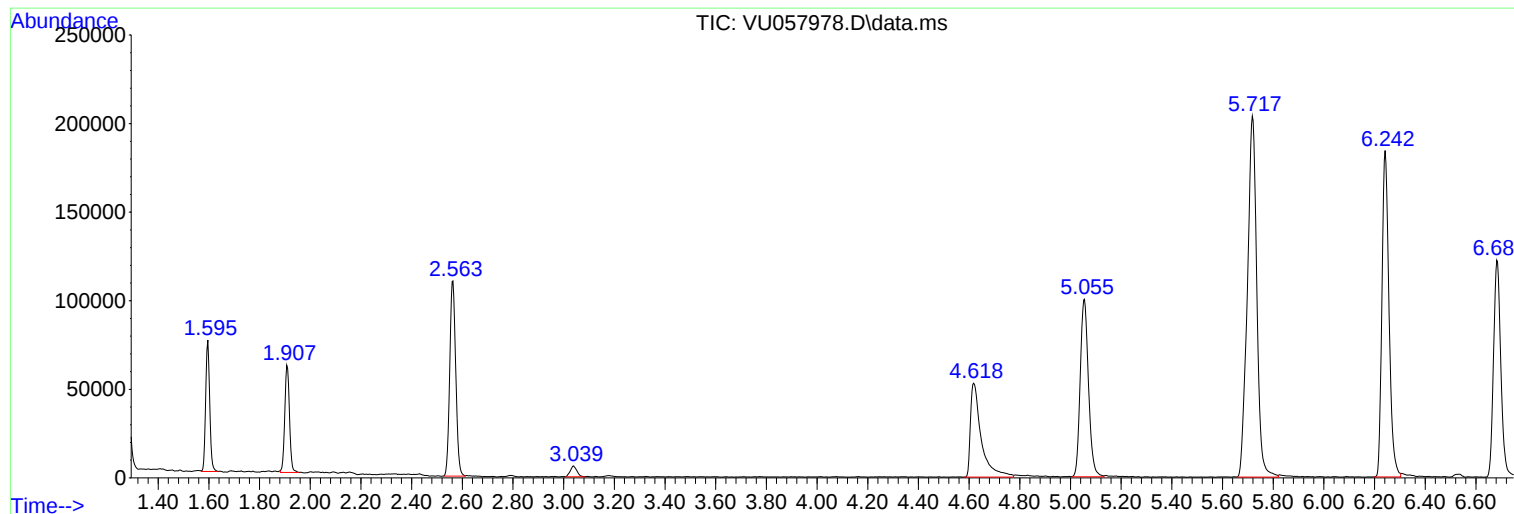

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030124\
Data File : VU057978.D
Acq On : 01 Mar 2024 12:15
Operator : MD/SY
Sample : VU0301WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK141

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030124\
Data File : VU057978.D
Acq On : 01 Mar 2024 12:15
Operator : MD/SY
Sample : VU0301WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK141

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc