
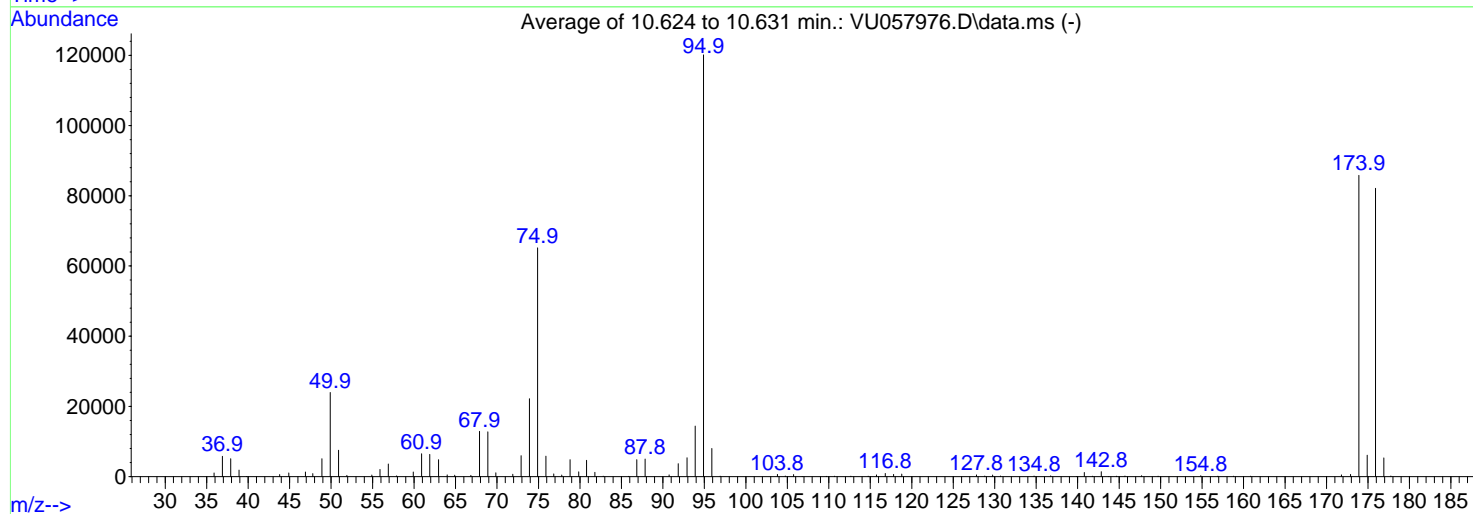


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030124\
 Data File : VU057976.D
 Acq On : 01 Mar 2024 09:34
 Operator : MD/SY
 Sample : BFB116
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB116

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Mar 01 22:42:28 2024

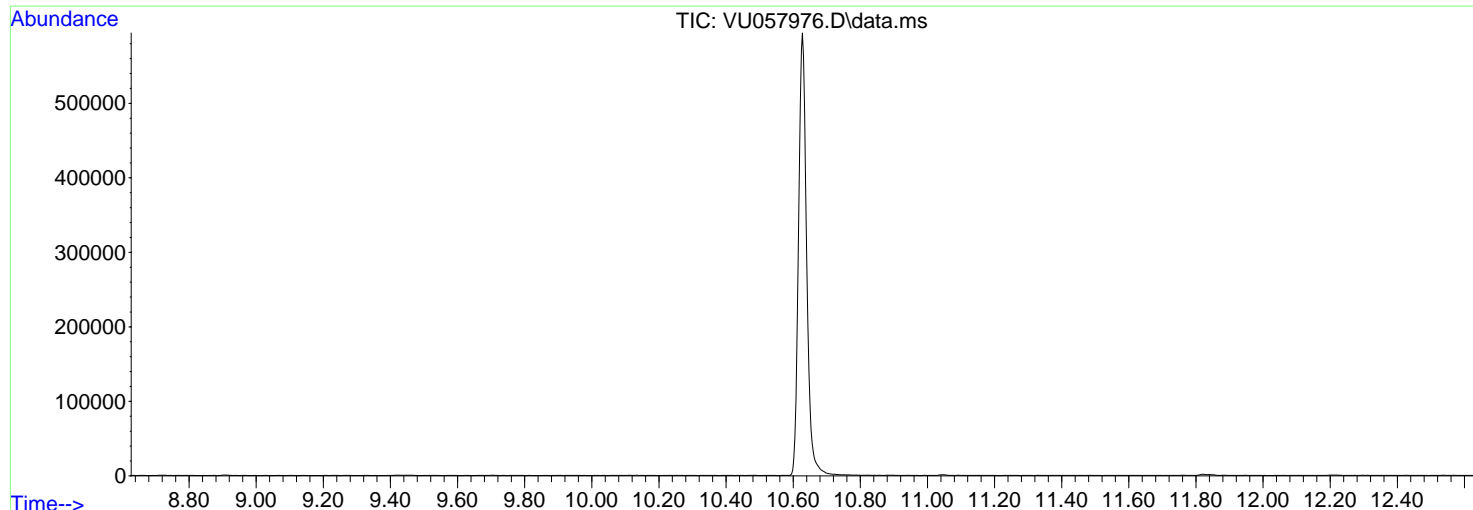

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	23965	PASS
75	95	30	80	54.2	65155	PASS
95	95	100	100	100.0	120144	PASS
96	95	5	9	6.7	8001	PASS
173	174	0.00	2	0.7	638	PASS
174	95	50	120	71.4	85819	PASS
175	174	5	9	7.1	6088	PASS
176	174	95	101	95.7	82139	PASS
177	176	5	9	6.5	5344	PASS

m/z	Abundance
39.90	268.0
43.80	447.0

Instrument :
MSVOA_U
ClientSampleId :
BFB116

m/z	Abundance
35.90	989.0
36.90	5974.0
37.90	5133.0
38.90	1797.0
39.80	309.0
43.80	1091.0
44.90	1095.0
46.90	1359.0
47.80	826.0
48.90	5369.0
49.90	24032.0
50.90	7588.0
51.90	339.0
54.90	444.0
55.90	2083.0
56.90	3937.0
57.90	243.0
59.90	1329.0
60.90	6556.0
61.90	6446.0
62.90	4919.0
64.00	498.0
64.90	448.0
66.90	323.0
67.90	13042.0
68.90	12903.0
69.80	1193.0
71.90	777.0
72.90	6159.0
73.90	22088.0
74.90	65144.0
75.90	5937.0
76.80	807.0
77.80	483.0
78.80	4754.0
79.80	1452.0
80.80	4711.0
81.80	1177.0
82.80	129.0
85.80	146.0
86.80	5028.0
87.80	5004.0
90.70	488.0
91.80	3697.0
92.90	5350.0
93.90	14474.0
94.90	119144.0
95.90	7925.0
96.90	146.0
103.80	590.0
104.70	179.0
105.80	640.0
106.80	100.0
110.70	145.0
112.60	139.0
114.80	148.0
115.70	501.0
116.80	929.0
117.80	652.0
118.80	707.0
127.80	504.0
128.80	212.0
129.80	387.0
130.70	203.0
134.70	197.0
136.80	221.0
140.80	1203.0
141.90	115.0
142.80	1401.0
144.70	174.0
145.70	198.0
147.70	293.0
149.70	106.0
154.80	263.0
156.90	136.0
158.80	138.0
160.80	119.0
171.80	563.0
172.90	693.0
173.90	82832.0
174.90	6151.0
175.90	79872.0
176.90	5194.0
177.80	169.0

Instrument :
MSVOA_U
ClientSampleId :
BFB116

m/z	Abundance
35.90	1043.0
36.90	5962.0
37.90	5238.0
38.90	1878.0
39.80	306.0
43.80	1092.0
44.90	1088.0
46.90	1330.0
47.80	895.0
48.90	5256.0
49.90	24792.0
50.90	7708.0
51.90	389.0
54.90	510.0
55.90	2106.0
56.90	3695.0
57.90	236.0
59.90	1359.0
60.90	6714.0
61.90	6621.0
63.00	5003.0
64.00	519.0
64.90	433.0
66.90	380.0
67.90	13379.0
68.90	13119.0
69.90	1134.0
71.90	734.0
72.90	6119.0
73.90	22864.0
74.90	67440.0
75.90	6081.0
76.80	778.0
77.80	473.0
78.80	4917.0
79.90	1402.0
80.80	4813.0
81.80	1289.0
82.80	141.0
85.90	105.0
86.80	4994.0
87.90	5229.0
90.80	530.0
91.90	3854.0
92.90	5596.0
93.90	14769.0
94.90	123848.0
95.90	8284.0
96.90	168.0
103.80	664.0
104.70	174.0
105.80	624.0
106.80	106.0
109.70	107.0
110.70	166.0
112.70	150.0
114.70	163.0
115.80	538.0
116.80	975.0
117.80	694.0
118.80	718.0
127.80	543.0
128.80	215.0
129.70	459.0
130.70	226.0
134.80	205.0
136.70	232.0
139.90	104.0
140.80	1230.0
141.80	158.0
142.90	1409.0
143.80	100.0
144.70	162.0
145.70	185.0
147.70	301.0
149.70	152.0
154.90	283.0
156.90	162.0
158.80	145.0
160.90	113.0
171.80	534.0
172.90	658.0
173.90	88392.0
174.90	6307.0
175.90	84696.0
176.90	5514.0
177.70	184.0

Instrument :
MSVOA_U
ClientSampleId :
BFB116

m/z	Abundance
35.90	1066.0
36.90	5446.0
37.90	4948.0
38.90	1911.0
39.80	318.0
43.80	961.0
44.90	1034.0
46.90	1344.0
47.80	846.0
48.90	4702.0
49.90	23072.0
50.90	7204.0
51.90	368.0
54.90	449.0
55.90	1950.0
56.90	3240.0
57.90	173.0
59.90	1262.0
60.90	6266.0
61.90	5975.0
62.90	4635.0
64.00	530.0
64.90	401.0
66.80	383.0
67.90	12230.0
68.90	12216.0
69.90	995.0
71.90	599.0
72.90	5682.0
73.90	21656.0
74.90	62880.0
75.90	5513.0
76.90	690.0
77.80	425.0
78.80	4765.0
79.90	1288.0
80.80	4485.0
81.80	1194.0
82.80	135.0
86.90	4426.0
87.90	4859.0
90.80	522.0
91.90	3591.0
92.90	5262.0
93.90	13944.0
94.90	117440.0
95.90	7795.0
96.90	168.0
103.80	644.0
104.80	172.0
105.70	575.0
109.70	114.0
110.70	171.0
112.70	147.0
114.70	153.0
115.80	520.0
116.80	860.0
117.80	592.0
118.80	728.0
127.80	489.0
128.80	195.0
129.70	466.0
130.70	189.0
134.70	199.0
136.70	224.0
140.80	1159.0
141.70	181.0
142.90	1394.0
143.70	105.0
144.70	114.0
145.70	167.0
147.70	292.0
149.70	168.0
154.90	293.0
156.90	148.0
158.80	136.0
160.80	122.0
171.80	464.0
172.90	563.0
173.90	86232.0
174.90	5807.0
175.90	81848.0
176.90	5325.0
177.70	164.0

Instrument :
MSVOA_U
ClientSampleId :
BFB116