

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU030220\
 Data File : VU036992.D
 Acq On : 02 Mar 2020 12:38
 Operator : JC/MD
 Sample : L1730-12
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	78	85	101	rVB	140720	151086	13.56%	1.808%
2	1.929	175	183	199	rVB	126040	165348	14.84%	1.978%
3	2.591	377	389	407	rBV	210738	346573	31.10%	4.147%
4	2.793	448	452	455	rBV2	251	183	0.02%	0.002%
5	2.845	465	468	469	rBV	158	65	0.01%	0.001%
6	2.990	510	513	514	rVB2	296	135	0.01%	0.002%
7	3.051	530	532	536	rVB	170	78	0.01%	0.001%
8	3.076	536	540	549	rBV3	405	521	0.05%	0.006%
9	3.112	549	551	554	rBV2	213	122	0.01%	0.001%
10	3.269	596	600	607	rVB2	288	289	0.03%	0.003%
11	3.302	607	610	611	rBV	166	74	0.01%	0.001%
12	3.334	619	620	623	rVB	212	103	0.01%	0.001%
13	3.363	625	629	632	rVB2	246	192	0.02%	0.002%
14	3.395	632	639	642	rBV	312	368	0.03%	0.004%
15	3.433	649	651	652	rBB	72	59	0.01%	0.001%
16	3.462	657	660	663	rVB	247	129	0.01%	0.002%
17	3.491	666	669	672	rVB2	191	109	0.01%	0.001%
18	3.511	672	675	677	rBV	100	56	0.01%	0.001%
19	3.536	677	683	687	rBV2	206	236	0.02%	0.003%
20	3.556	687	689	693	rVB	142	73	0.01%	0.001%
21	3.633	710	713	715	rBV	129	78	0.01%	0.001%
22	3.674	719	726	729	rBV2	322	288	0.03%	0.003%
23	3.716	736	739	743	rVB	290	188	0.02%	0.002%
24	3.739	743	746	750	rBV	242	203	0.02%	0.002%
25	3.771	752	756	758	rBV	118	97	0.01%	0.001%
26	3.810	764	768	770	rBV	104	83	0.01%	0.001%
27	3.986	821	823	827	rVB	172	65	0.01%	0.001%
28	4.009	827	830	836	rVB	230	228	0.02%	0.003%
29	4.047	839	842	844	rVB	180	80	0.01%	0.001%
30	4.067	844	848	852	rBV2	155	165	0.01%	0.002%
31	4.105	856	860	863	rBV2	173	194	0.02%	0.002%
32	4.147	870	873	877	rVB2	206	160	0.01%	0.002%
33	4.189	883	886	889	rBV2	171	141	0.01%	0.002%
34	4.250	902	905	907	rBV	213	145	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU030220\
 Data File : VU036992.D
 Acq On : 02 Mar 2020 12:38
 Operator : JC/MD
 Sample : L1730-12
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
 Title : VOC Analysis

35	4.282	913	915	917	rVB	161	65	0.01%	0.001%
36	4.318	922	926	930	rVB2	269	227	0.02%	0.003%
37	4.343	931	934	938	rBV	230	214	0.02%	0.003%
38	4.459	965	970	974	rBV	221	168	0.02%	0.002%
39	4.568	999	1004	1006	rBV	212	121	0.01%	0.001%
40	4.617	1016	1019	1020	rBV	172	112	0.01%	0.001%
41	4.668	1020	1035	1067	rVV	118785	280668	25.19%	3.358%
42	5.105	1154	1171	1193	rBV	190985	421315	37.81%	5.041%
43	5.256	1216	1218	1220	rBV2	207	152	0.01%	0.002%
44	5.311	1230	1235	1237	rBV3	680	585	0.05%	0.007%
45	5.404	1260	1264	1265	rBV2	422	265	0.02%	0.003%
46	5.446	1273	1277	1278	rBV	215	153	0.01%	0.002%
47	5.539	1299	1306	1310	rBV2	217	274	0.02%	0.003%
48	5.559	1310	1312	1316	rBV	180	174	0.02%	0.002%
49	5.761	1353	1375	1396	rBV2	423030	1114272	100.00%	13.332%
50	5.996	1444	1448	1452	rBV3	382	355	0.03%	0.004%
51	6.199	1506	1511	1514	rVB2	273	211	0.02%	0.003%
52	6.227	1517	1520	1522	rBV	144	77	0.01%	0.001%
53	6.282	1522	1537	1559	rBV	354270	658116	59.06%	7.874%
54	6.411	1575	1577	1582	rBV2	432	336	0.03%	0.004%
55	6.559	1612	1623	1640	rVB4	3947	6781	0.61%	0.081%
56	6.620	1640	1642	1646	rBV2	217	141	0.01%	0.002%
57	6.645	1647	1650	1654	rVB	152	67	0.01%	0.001%
58	6.723	1656	1674	1693	rBV	267308	520945	46.75%	6.233%
59	6.899	1727	1729	1732	rBV2	129	78	0.01%	0.001%
60	6.941	1739	1742	1746	rBV2	263	241	0.02%	0.003%
61	6.964	1747	1749	1753	rVB2	293	155	0.01%	0.002%
62	6.989	1753	1757	1764	rBV2	262	337	0.03%	0.004%
63	7.025	1764	1768	1772	rBV2	179	189	0.02%	0.002%
64	7.076	1777	1784	1786	rVB	251	264	0.02%	0.003%
65	7.096	1786	1790	1791	rBV	171	119	0.01%	0.001%
66	7.157	1805	1809	1811	rBV2	198	162	0.01%	0.002%
67	7.285	1846	1849	1853	rBV2	223	157	0.01%	0.002%
68	7.379	1873	1878	1880	rBV2	222	209	0.02%	0.003%
69	7.594	1932	1945	1968	rBV	144567	254845	22.87%	3.049%
70	7.790	2003	2006	2009	rBV2	346	308	0.03%	0.004%
71	7.848	2022	2024	2028	rBV	230	187	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU030220\
 Data File : VU036992.D
 Acq On : 02 Mar 2020 12:38
 Operator : JC/MD
 Sample : L1730-12
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
 Title : VOC Analysis

72	7.925	2033	2048	2068	rBV	520651	899104	80.69%	10.758%
73	8.205	2122	2135	2154	rBV	100238	170248	15.28%	2.037%
74	8.337	2173	2176	2187	rVB4	572	701	0.06%	0.008%
75	8.395	2192	2194	2197	rBV2	209	137	0.01%	0.002%
76	8.491	2222	2224	2225	rBV2	193	54	0.00%	0.001%
77	8.658	2263	2276	2328	rBV	328472	638490	57.30%	7.640%
78	9.083	2406	2408	2411	rVB2	209	135	0.01%	0.002%
79	9.121	2415	2420	2424	rBV2	328	401	0.04%	0.005%
80	9.324	2479	2483	2485	rBV	278	248	0.02%	0.003%
81	9.366	2493	2496	2497	rBV	198	116	0.01%	0.001%
82	9.440	2505	2519	2552	rBV	483003	807161	72.44%	9.658%
83	9.661	2583	2588	2592	rBV2	253	318	0.03%	0.004%
84	9.841	2641	2644	2647	rBV2	191	143	0.01%	0.002%
85	10.034	2701	2704	2707	rBV	210	179	0.02%	0.002%
86	10.349	2796	2802	2807	rBV2	231	262	0.02%	0.003%
87	10.677	2901	2904	2909	rBV2	210	217	0.02%	0.003%
88	10.774	2921	2934	2957	rVB	354190	574623	51.57%	6.875%
89	10.857	2957	2960	2962	rBV2	197	125	0.01%	0.001%
90	10.970	2994	2995	2998	rBV2	335	108	0.01%	0.001%
91	11.063	3022	3024	3026	rBV	246	136	0.01%	0.002%
92	11.102	3034	3036	3040	rBV2	284	175	0.02%	0.002%
93	11.285	3090	3093	3097	rBV	341	299	0.03%	0.004%
94	11.484	3153	3155	3158	rBV2	280	223	0.02%	0.003%
95	11.610	3188	3194	3195	rBV2	281	259	0.02%	0.003%
96	11.642	3200	3204	3206	rBV2	291	225	0.02%	0.003%
97	11.829	3249	3262	3280	rVB	380319	632159	56.73%	7.564%
98	11.941	3294	3297	3300	rBV	319	254	0.02%	0.003%
99	12.208	3368	3380	3397	rBV	425086	699945	62.82%	8.375%
100	13.761	3860	3863	3865	rBV	309	232	0.02%	0.003%


Sum of corrected areas: 8357636

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU030220\
Data File : VU036992.D
Acq On : 02 Mar 2020 12:38
Operator : JC/MD
Sample : L1730-12
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

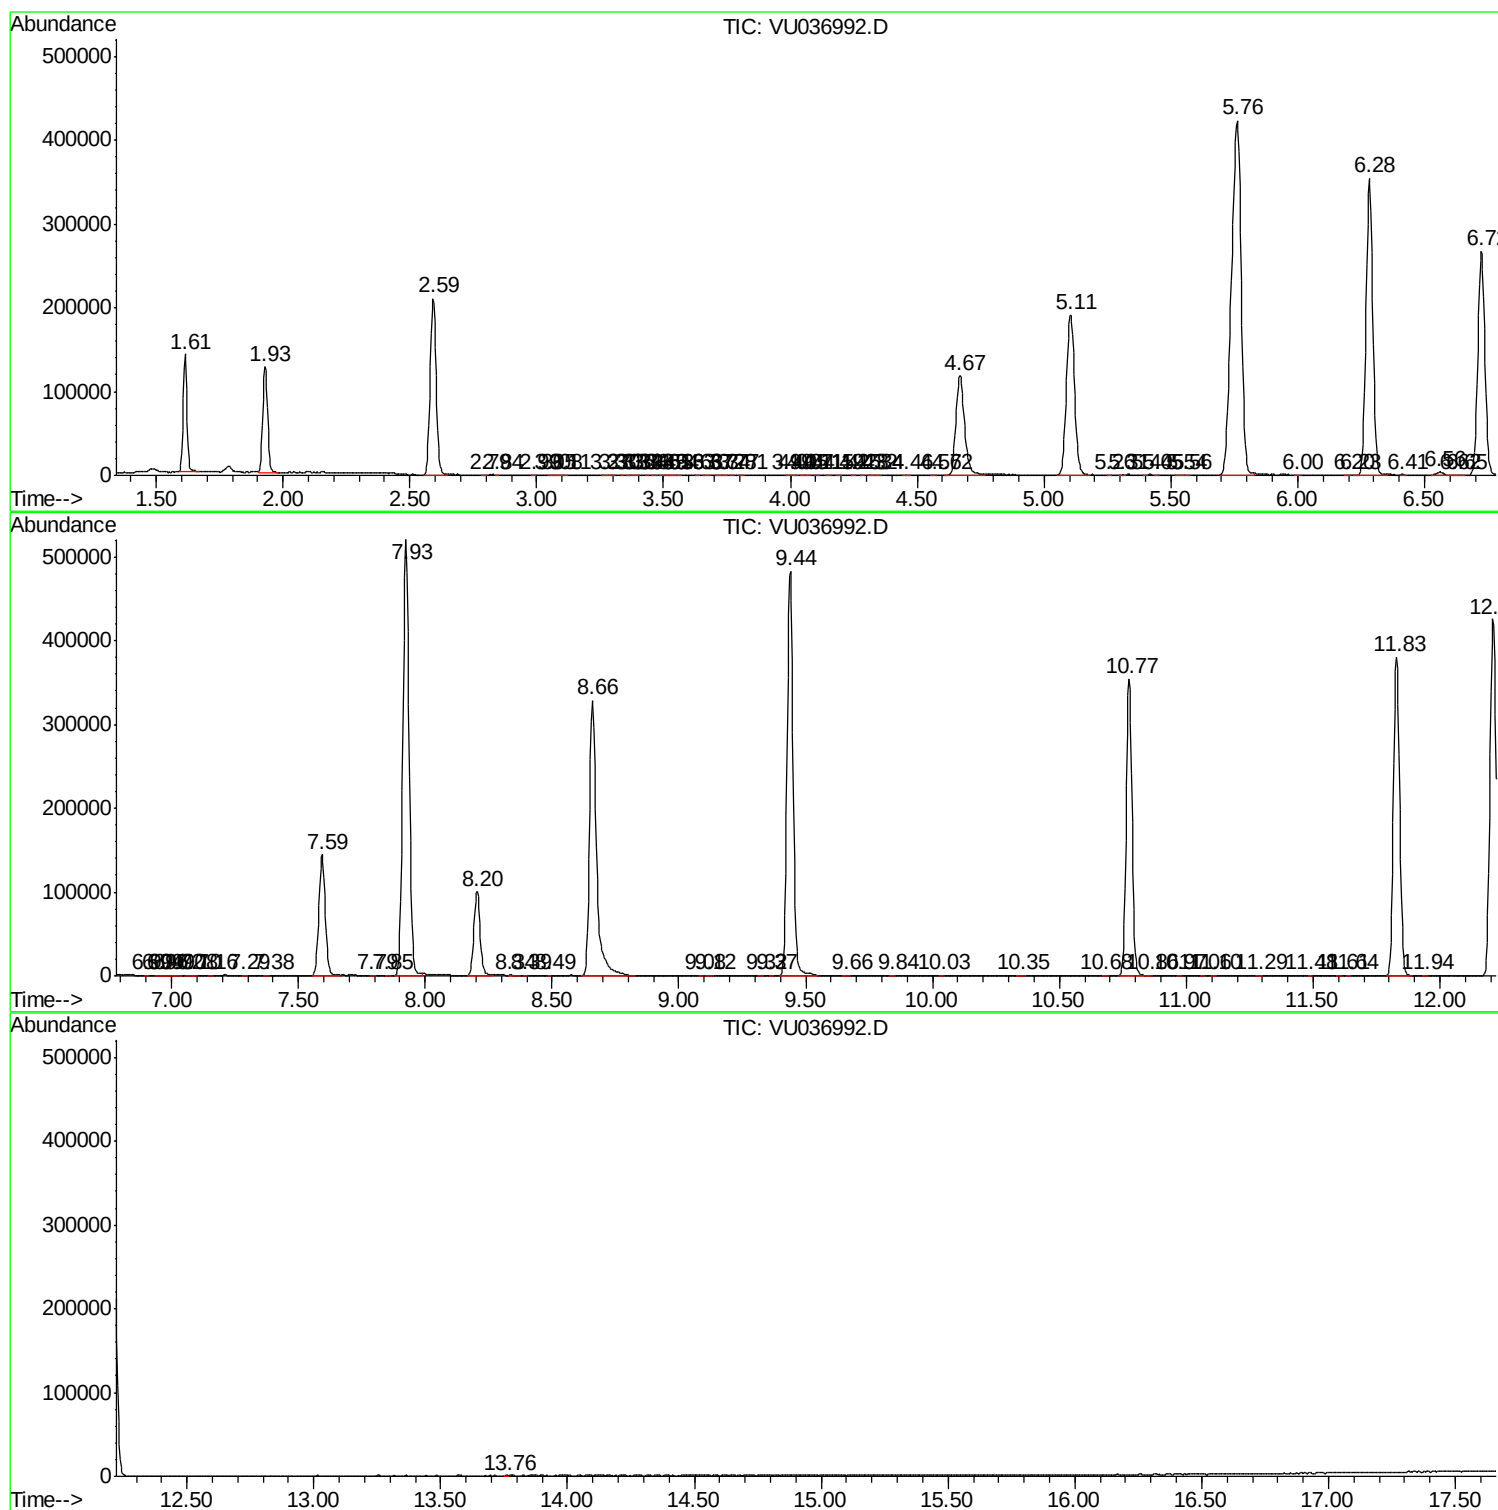

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU030220\
Data File : VU036992.D
Acq On : 02 Mar 2020 12:38
Operator : JC/MD
Sample : L1730-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU030220\
Data File : VU036992.D
Acq On : 02 Mar 2020 12:38
Operator : JC/MD
Sample : L1730-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc