

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU030220\
 Data File : VU036993.D
 Acq On : 02 Mar 2020 13:01
 Operator : JC/MD
 Sample : L1708-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	78	85	96	rBV	135650	144703	13.34%	1.783%
2	1.929	176	183	194	rVB	118679	152373	14.05%	1.877%
3	2.591	377	389	408	rBV	200711	331509	30.57%	4.084%
4	3.038	525	528	532	rBV2	214	201	0.02%	0.002%
5	3.125	552	555	557	rBV2	198	154	0.01%	0.002%
6	3.154	561	564	567	rBV2	283	246	0.02%	0.003%
7	3.353	623	626	629	rBV	258	215	0.02%	0.003%
8	3.420	644	647	654	rVB2	279	360	0.03%	0.004%
9	3.459	654	659	662	rBV2	324	385	0.04%	0.005%
10	3.543	683	685	689	rVB	188	85	0.01%	0.001%
11	3.623	708	710	714	rBV2	202	161	0.01%	0.002%
12	3.710	735	737	738	rBV	132	54	0.00%	0.001%
13	3.858	781	783	787	rVB	140	65	0.01%	0.001%
14	3.883	787	791	793	rBV2	201	144	0.01%	0.002%
15	3.912	798	800	803	rVB2	178	100	0.01%	0.001%
16	3.938	805	808	811	rVB	142	82	0.01%	0.001%
17	3.954	811	813	818	rBV2	183	157	0.01%	0.002%
18	4.054	842	844	847	rBV2	182	109	0.01%	0.001%
19	4.154	871	875	878	rBV2	213	168	0.02%	0.002%
20	4.173	878	881	886	rVV	190	220	0.02%	0.003%
21	4.263	907	909	912	rBV	167	114	0.01%	0.001%
22	4.359	937	939	940	rBV	125	50	0.00%	0.001%
23	4.379	940	945	949	rBV2	272	254	0.02%	0.003%
24	4.462	969	971	972	rBV2	119	52	0.00%	0.001%
25	4.504	983	984	986	rBV2	84	39	0.00%	0.000%
26	4.533	989	993	997	rVB2	250	241	0.02%	0.003%
27	4.562	997	1002	1004	rBV	254	240	0.02%	0.003%
28	4.607	1014	1016	1017	rBV	176	79	0.01%	0.001%
29	4.668	1020	1035	1063	rBV	119141	282039	26.01%	3.474%
30	5.105	1155	1171	1193	rBV	183415	408502	37.67%	5.032%
31	5.224	1206	1208	1209	rBV	223	128	0.01%	0.002%
32	5.266	1219	1221	1225	rBV2	234	131	0.01%	0.002%
33	5.330	1233	1241	1247	rBV3	819	1138	0.10%	0.014%
34	5.407	1260	1265	1266	rBV	511	433	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU030220\
 Data File : VU036993.D
 Acq On : 02 Mar 2020 13:01
 Operator : JC/MD
 Sample : L1708-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
 Title : VOC Analysis

35	5.443	1273	1276	1278	rBV2	149	105	0.01%	0.001%
36	5.485	1287	1289	1292	rVB2	191	117	0.01%	0.001%
37	5.575	1315	1317	1320	rBV	199	140	0.01%	0.002%
38	5.652	1338	1341	1348	rVB2	260	299	0.03%	0.004%
39	5.684	1348	1351	1353	rBV2	313	151	0.01%	0.002%
40	5.761	1353	1375	1397	rBV2	408623	1084509	100.00%	13.360%
41	6.083	1473	1475	1483	rVB3	523	464	0.04%	0.006%
42	6.231	1518	1521	1522	rBV	204	114	0.01%	0.001%
43	6.282	1522	1537	1558	rVV	337218	630926	58.18%	7.772%
44	6.559	1614	1623	1633	rBV5	3697	5938	0.55%	0.073%
45	6.723	1656	1674	1692	rBV	262587	503635	46.44%	6.204%
46	6.909	1729	1732	1734	rBV2	306	203	0.02%	0.003%
47	6.925	1734	1737	1740	rVB	274	174	0.02%	0.002%
48	6.977	1750	1753	1755	rVB	210	110	0.01%	0.001%
49	6.999	1755	1760	1763	rBV	280	251	0.02%	0.003%
50	7.157	1806	1809	1811	rBV	183	92	0.01%	0.001%
51	7.256	1837	1840	1841	rBV	184	115	0.01%	0.001%
52	7.350	1864	1869	1871	rBV	126	132	0.01%	0.002%
53	7.366	1871	1874	1878	rVV	276	230	0.02%	0.003%
54	7.404	1885	1886	1888	rVB	148	49	0.00%	0.001%
55	7.475	1905	1908	1911	rBV	171	95	0.01%	0.001%
56	7.497	1911	1915	1918	rBV	169	189	0.02%	0.002%
57	7.536	1925	1927	1929	rBV	196	78	0.01%	0.001%
58	7.591	1932	1944	1963	rVV	141158	245665	22.65%	3.026%
59	7.925	2033	2048	2065	rBV	496588	860658	79.36%	10.602%
60	8.202	2122	2134	2156	rBV	96168	166656	15.37%	2.053%
61	8.446	2208	2210	2215	rVB2	215	184	0.02%	0.002%
62	8.491	2215	2224	2231	rBV2	349	552	0.05%	0.007%
63	8.555	2240	2244	2248	rBV2	243	301	0.03%	0.004%
64	8.658	2263	2276	2328	rBV	328341	642490	59.24%	7.915%
65	8.893	2346	2349	2350	rBV	112	75	0.01%	0.001%
66	9.018	2384	2388	2393	rBV	313	368	0.03%	0.005%
67	9.292	2471	2473	2475	rBV	164	75	0.01%	0.001%
68	9.330	2482	2485	2487	rBV	303	213	0.02%	0.003%
69	9.436	2505	2518	2555	rVB	467792	786063	72.48%	9.683%
70	9.565	2555	2558	2562	rBV2	226	216	0.02%	0.003%
71	9.629	2575	2578	2581	rBV	197	160	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU030220\
 Data File : VU036993.D
 Acq On : 02 Mar 2020 13:01
 Operator : JC/MD
 Sample : L1708-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
 Title : VOC Analysis

72	9.845	2643	2645	2646	rBV	188	63	0.01%	0.001%
73	10.140	2734	2737	2739	rBV2	201	117	0.01%	0.001%
74	10.349	2800	2802	2804	rBV	152	102	0.01%	0.001%
75	10.665	2897	2900	2901	rBV	232	114	0.01%	0.001%
76	10.703	2908	2912	2916	rBV2	322	337	0.03%	0.004%
77	10.774	2922	2934	2956	rVB	348757	564878	52.09%	6.959%
78	11.044	3012	3018	3020	rBV2	337	354	0.03%	0.004%
79	11.105	3034	3037	3039	rBV	324	210	0.02%	0.003%
80	11.137	3044	3047	3050	rBV	248	193	0.02%	0.002%
81	11.173	3055	3058	3061	rBV2	229	183	0.02%	0.002%
82	11.420	3130	3135	3138	rBV2	313	345	0.03%	0.004%
83	11.828	3250	3262	3281	rVB	365080	610672	56.31%	7.523%
84	12.076	3336	3339	3343	rBV2	289	308	0.03%	0.004%
85	12.208	3367	3380	3395	rBV	413860	682442	62.93%	8.407%
86	12.359	3425	3427	3432	rBV2	255	130	0.01%	0.002%
87	12.655	3513	3519	3521	rBV	420	406	0.04%	0.005%


Sum of corrected areas: 8117577

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU030220\
Data File : VU036993.D
Acq On : 02 Mar 2020 13:01
Operator : JC/MD
Sample : L1708-07
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

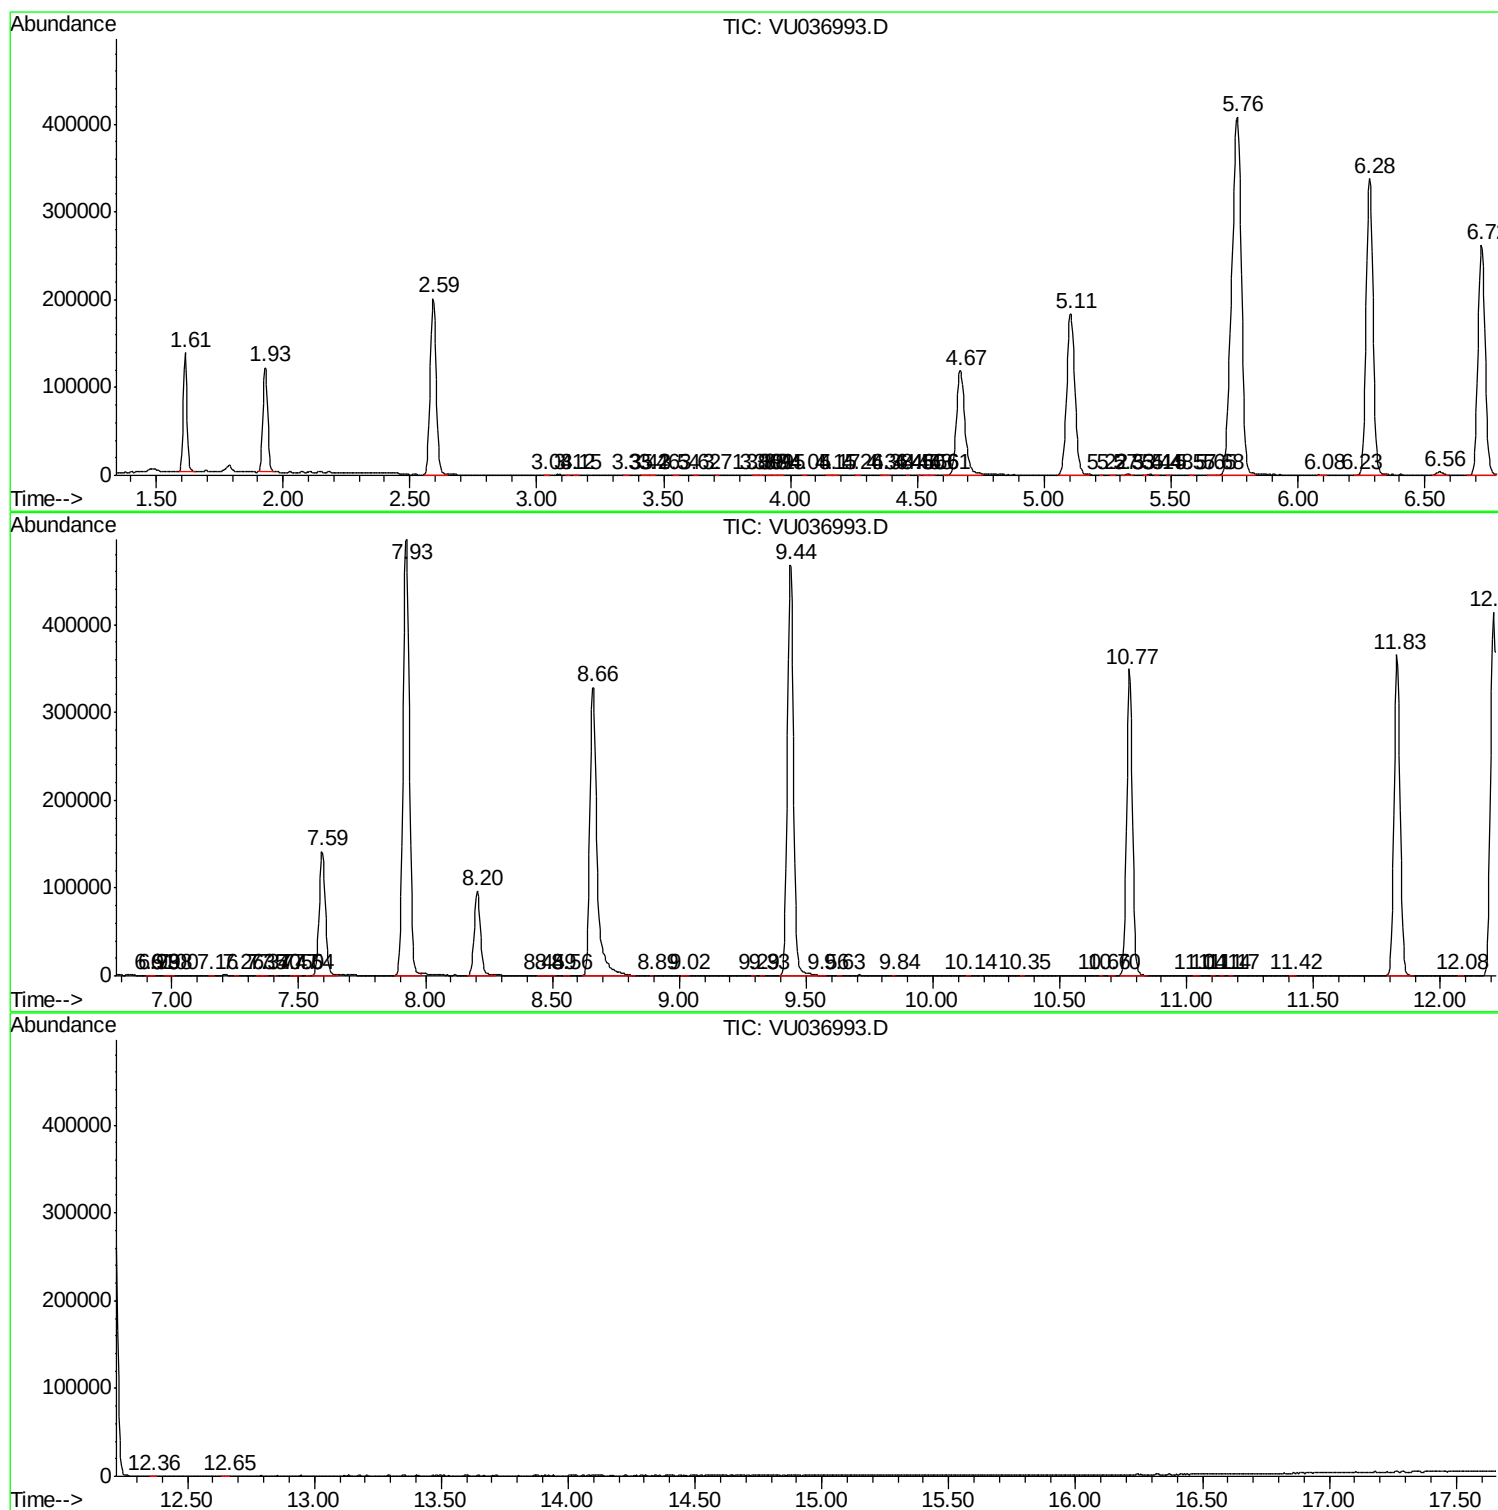

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU030220\
Data File : VU036993.D
Acq On : 02 Mar 2020 13:01
Operator : JC/MD
Sample : L1708-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU030220\
Data File : VU036993.D
Acq On : 02 Mar 2020 13:01
Operator : JC/MD
Sample : L1708-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc