


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU030220\
 Data File : VU036988.D
 Acq On : 02 Mar 2020 10:33
 Operator : JC/MD
 Sample : BFB55
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB55

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
 Title : VOC Analysis
 Last Update : Tue Mar 03 03:21:45 2020

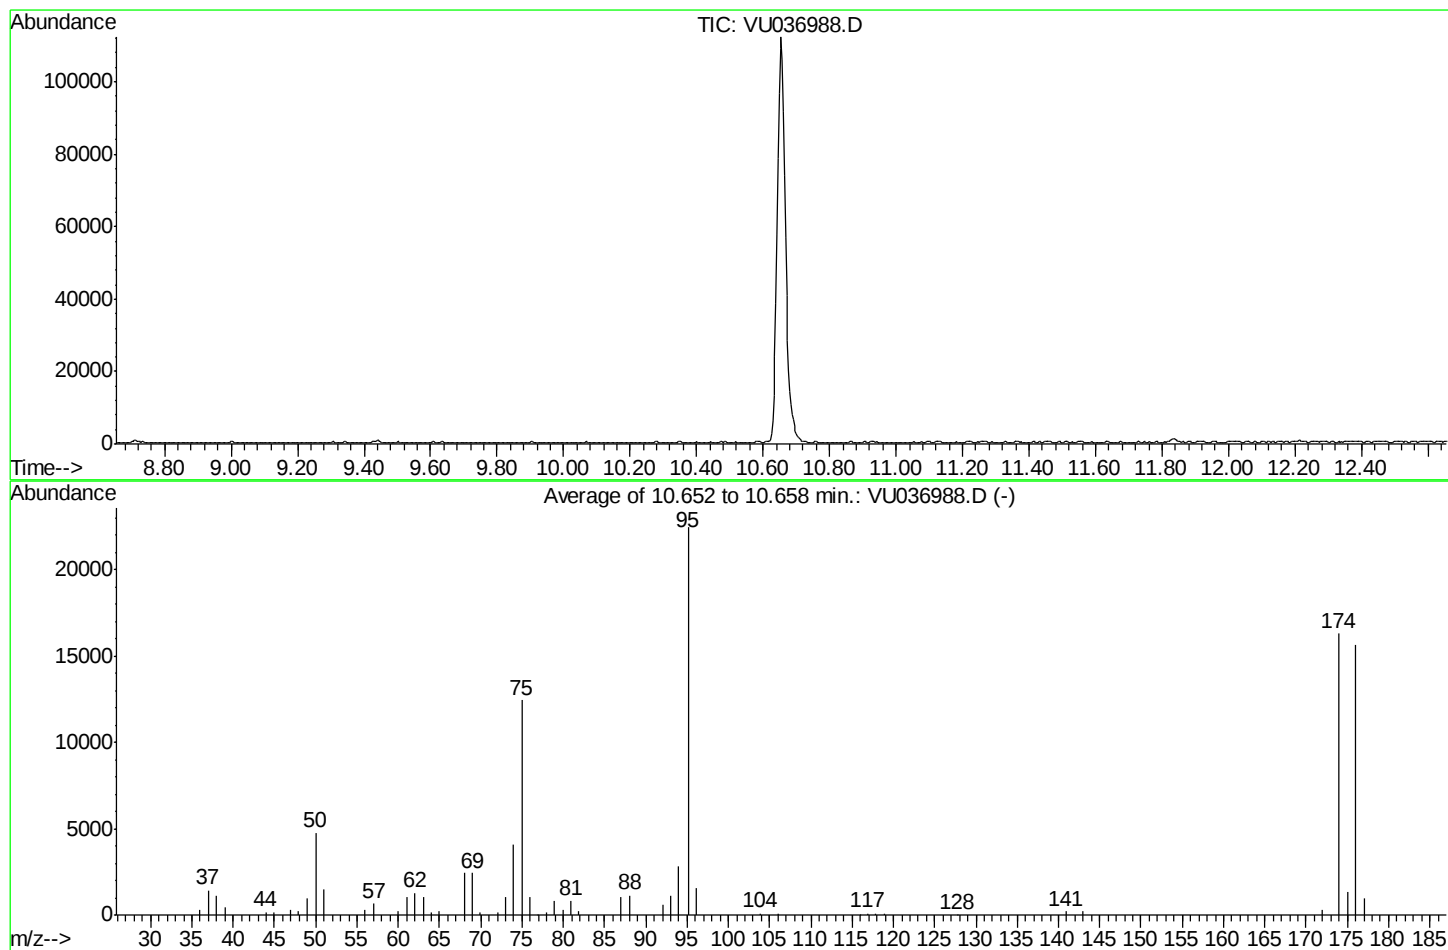

AutoFind: Scans 2896, 2897, 2898; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	4771	PASS
75	95	30	80	55.4	12439	PASS
95	95	100	100	100.0	22448	PASS
96	95	5	9	6.8	1532	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.5	16284	PASS
175	174	5	9	8.4	1373	PASS
176	174	95	101	95.9	15617	PASS
177	176	5	9	6.0	936	PASS

m/z	Abundance
35.00	318.0
37.00	1490.0
37.90	1132.0
39.00	473.0
40.00	149.0
44.00	539.0
45.00	166.0
47.00	267.0
47.90	175.0
49.00	948.0
50.00	4985.0
51.00	1450.0
56.00	358.0
57.00	683.0
60.00	254.0
61.00	1039.0
62.00	1275.0
63.00	1079.0
63.90	187.0
65.00	226.0
68.00	2557.0
69.00	2409.0
69.90	190.0
72.00	158.0
73.00	1170.0
74.00	4111.0
75.00	12498.0
76.00	1069.0
77.90	124.0
79.00	880.0
79.90	333.0
81.00	843.0
81.90	235.0
86.90	1052.0
88.10	1121.0
92.00	645.0
93.00	1068.0
94.00	2759.0
95.10	22392.0
96.10	1631.0
103.90	100.0
106.00	123.0
117.00	118.0
127.80	101.0
141.00	229.0
143.00	199.0
171.90	230.0
174.00	15905.0
175.00	1335.0
176.00	15379.0
177.00	966.0

Instrument :
MSVOA_U
ClientSampleId :
BFB55

m/z	Abundance
35.90	308.0
37.00	1518.0
37.90	1178.0
39.00	463.0
40.00	147.0
44.00	612.0
44.90	164.0
47.00	286.0
47.90	206.0
48.90	997.0
50.00	4968.0
51.00	1540.0
56.00	338.0
57.00	657.0
59.90	226.0
61.00	1051.0
62.00	1312.0
63.00	1097.0
63.90	175.0
65.00	240.0
68.00	2483.0
69.00	2522.0
69.90	195.0
72.00	168.0
73.00	1086.0
74.00	4157.0
75.00	12839.0
76.00	1079.0
77.90	110.0
79.00	844.0
79.90	296.0
81.00	874.0
81.90	246.0
87.00	1064.0
88.00	1182.0
92.00	615.0
93.00	1118.0
94.00	2850.0
95.10	23120.0
96.10	1563.0
103.90	108.0
116.00	105.0
116.90	109.0
117.80	118.0
118.90	130.0
141.00	230.0
142.90	191.0
172.00	329.0
174.00	16840.0
175.00	1397.0
176.00	16016.0
177.00	908.0

Instrument :
MSVOA_U
ClientSampleId :
BFB55

m/z	Abundance
35.90	283.0
37.00	1331.0
38.00	1076.0
39.00	436.0
39.90	126.0
44.00	656.0
44.90	182.0
46.90	266.0
47.90	199.0
48.90	1020.0
50.00	4361.0
51.00	1436.0
55.90	288.0
57.10	598.0
59.90	202.0
61.00	1018.0
62.00	1214.0
63.00	1018.0
64.00	134.0
65.00	205.0
68.00	2275.0
69.00	2404.0
70.00	170.0
72.00	161.0
73.00	943.0
74.00	3878.0
75.00	11982.0
76.00	987.0
76.90	117.0
77.90	110.0
78.90	758.0
79.90	259.0
80.90	831.0
81.90	220.0
87.00	1016.0
88.00	1148.0
92.00	565.0
93.00	1065.0
94.00	2761.0
95.10	21832.0
96.10	1404.0
103.90	105.0
116.90	104.0
117.80	124.0
118.90	162.0
141.00	208.0
142.80	180.0
172.00	335.0
174.00	16107.0
175.00	1387.0
176.00	15457.0
177.00	935.0

Instrument :
MSVOA_U
ClientSampleId :
BFB55

Scan 2884 (10.613 min): VU036988.D
BFB55

m/z	Abundance
39.90	165.0
43.90	415.0

Instrument :
MSVOA_U
ClientSampleId :
BFB55