


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030221\
Data File : VU042466.D
Acq On : 02 Mar 2021 11:17
Operator : SY/MD
Sample : BFB40
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB40

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Mar 05 00:31:48 2021

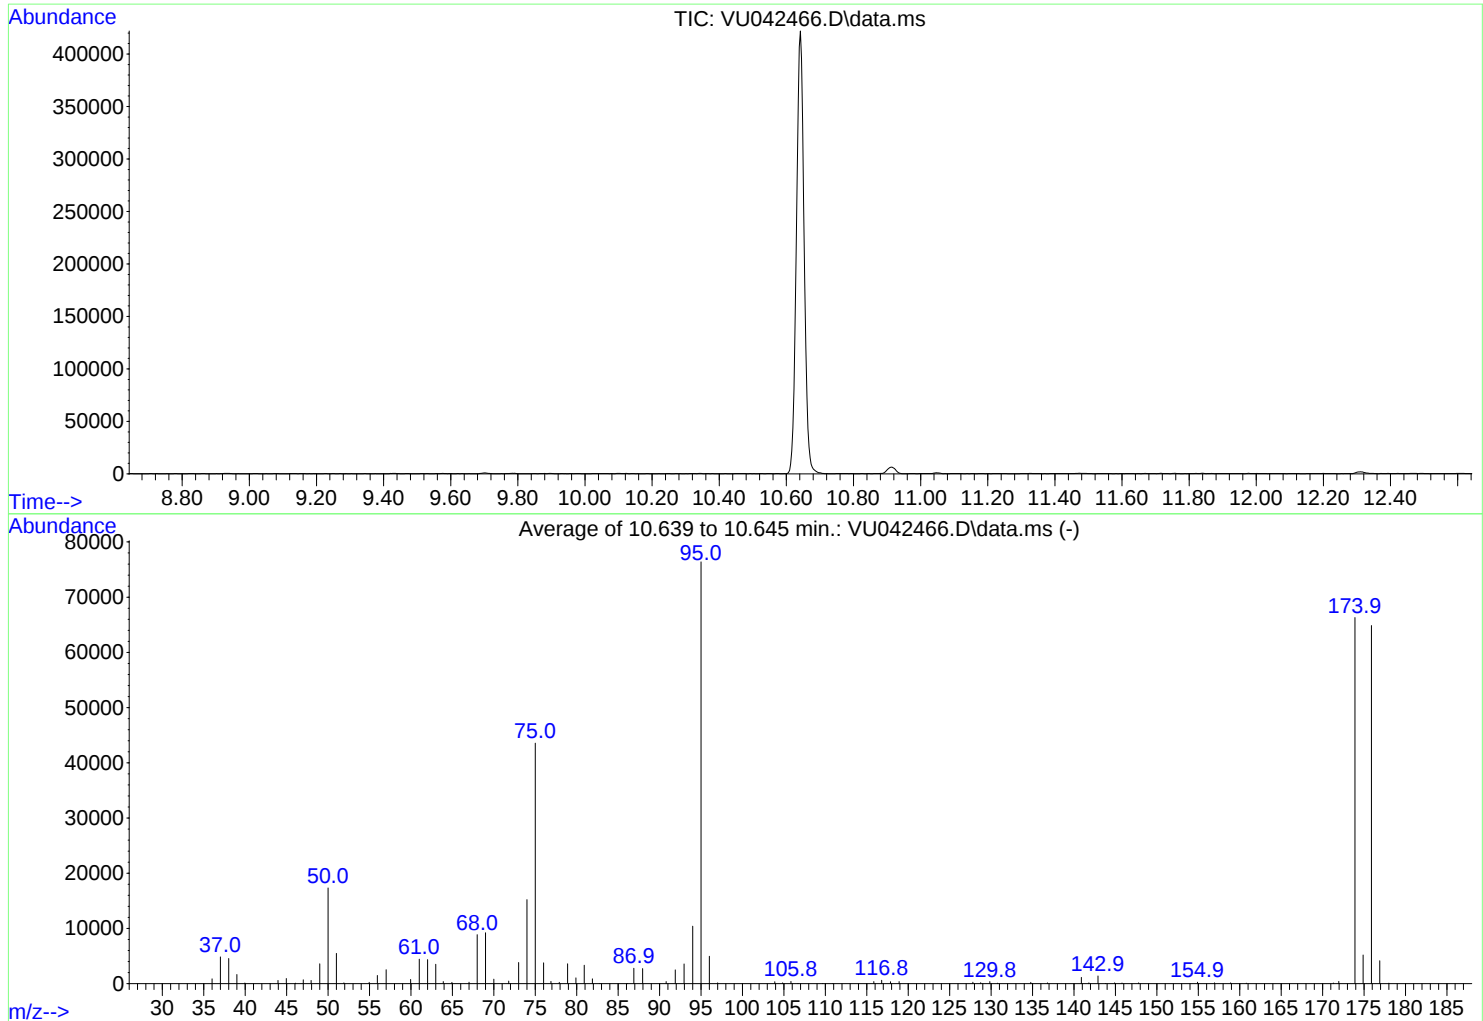

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	17323	PASS
75	95	30	80	57.0	43547	PASS
95	95	100	100	100.0	76397	PASS
96	95	5	9	6.5	4959	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	86.8	66315	PASS
175	174	5	9	7.8	5188	PASS
176	174	95	101	97.8	64851	PASS
177	176	5	9	6.4	4157	PASS

m/z	Abundance
36.00	842.0
37.00	4962.0
38.00	4611.0
39.00	1725.0
40.00	139.0
43.00	105.0
44.00	840.0
44.90	900.0
46.00	112.0
47.00	639.0
47.90	599.0
49.00	3750.0
50.00	17272.0
51.00	5589.0
51.90	179.0
55.00	261.0
55.90	1531.0
57.00	2560.0
59.90	746.0
61.00	4537.0
62.00	4254.0
63.00	3435.0
63.90	446.0
65.00	263.0
67.00	247.0
68.00	8793.0
69.00	9205.0
70.00	843.0
71.80	448.0
73.00	3911.0
74.00	15582.0
75.00	43920.0
76.00	3858.0
76.80	409.0
77.90	218.0
78.90	3545.0
79.90	1022.0
80.90	3375.0
81.90	956.0
86.90	2772.0
87.90	2694.0
90.80	359.0
91.90	2598.0
93.00	3558.0
94.00	10147.0
95.00	76952.0
96.00	4938.0
97.00	149.0
103.90	357.0
104.80	130.0
105.90	446.0
109.70	142.0
110.90	101.0
115.90	369.0
116.80	640.0
117.80	332.0
118.90	367.0
127.80	310.0
128.80	223.0
129.80	433.0
130.80	137.0
134.80	223.0
136.80	138.0
140.90	1123.0
141.80	155.0
142.90	1316.0
143.80	106.0
144.90	148.0
145.80	112.0
147.80	140.0
154.90	283.0
156.90	147.0
158.90	129.0
160.80	130.0
171.30	165.0
171.90	377.0
173.90	64736.0
174.90	5150.0
175.90	63024.0
176.90	4160.0
178.00	119.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.00	919.0
37.00	5040.0
38.00	4733.0
39.00	1683.0
40.00	113.0
44.00	862.0
44.90	976.0
46.10	121.0
47.00	699.0
48.00	585.0
49.00	3694.0
50.00	17984.0
51.00	5653.0
51.90	142.0
55.00	227.0
56.00	1544.0
57.00	2545.0
60.00	753.0
61.00	4587.0
62.00	4459.0
63.00	3681.0
63.90	382.0
64.90	245.0
67.00	265.0
68.00	9222.0
69.00	9590.0
70.00	847.0
71.80	506.0
73.00	3955.0
74.00	15624.0
75.00	44904.0
76.00	3932.0
76.90	393.0
77.90	268.0
78.90	3709.0
79.90	1083.0
80.90	3414.0
81.90	906.0
86.10	101.0
86.90	2837.0
87.90	2813.0
90.80	390.0
91.90	2562.0
92.90	3677.0
94.00	10756.0
95.00	79080.0
96.00	5106.0
97.00	164.0
103.90	377.0
104.80	147.0
105.80	410.0
115.90	391.0
116.80	632.0
117.80	349.0
118.90	390.0
127.80	284.0
128.70	179.0
129.80	378.0
130.80	117.0
134.80	244.0
136.80	125.0
140.90	1201.0
141.80	174.0
142.90	1471.0
144.90	153.0
145.80	131.0
147.80	167.0
154.90	279.0
157.00	160.0
158.90	151.0
160.80	127.0
171.30	200.0
172.00	403.0
173.90	68544.0
174.90	5372.0
175.90	67184.0
176.90	4302.0
178.00	118.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.00	868.0
37.00	4551.0
38.00	4317.0
39.00	1535.0
39.90	119.0
44.00	767.0
45.00	881.0
47.00	728.0
48.00	522.0
49.00	3360.0
50.00	16712.0
51.00	5219.0
51.90	142.0
54.90	203.0
56.00	1392.0
57.00	2427.0
60.00	757.0
61.00	4208.0
62.00	4321.0
63.00	3413.0
64.00	274.0
64.90	200.0
67.00	281.0
68.00	8554.0
69.00	8841.0
70.00	782.0
71.80	462.0
73.00	3661.0
74.00	14429.0
75.00	41816.0
76.00	3539.0
77.00	388.0
77.90	247.0
78.90	3489.0
79.90	1014.0
80.90	3233.0
81.90	796.0
82.80	108.0
86.90	2719.0
88.00	2682.0
90.80	358.0
91.90	2361.0
92.90	3485.0
94.00	10274.0
95.00	73160.0
96.00	4834.0
97.00	148.0
103.90	348.0
104.90	148.0
105.80	370.0
106.70	100.0
115.80	352.0
116.80	534.0
117.90	329.0
118.90	397.0
127.80	236.0
128.70	149.0
129.90	303.0
134.80	244.0
136.80	141.0
140.90	1090.0
141.80	143.0
142.90	1431.0
144.90	140.0
145.80	108.0
147.80	182.0
154.90	235.0
157.00	132.0
158.90	146.0
172.00	420.0
173.90	65664.0
174.90	5043.0
175.90	64344.0
176.90	4008.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
43.90	250.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40