

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
 Data File : VU053182.D
 Acq On : 02 Mar 2023 13:02
 Operator : JC/MD
 Sample : 01745-05DL 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0LF2DL

Quant Time: Mar 03 01:46:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 03 01:44:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.244	114	201127	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.411	117	190132	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	94046	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.598	65	65356	35.373	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	70.740%		
7) Chloroethane-d5	1.913	69	61662	39.433	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	78.860%		
11) 1,1-Dichloroethene-d2	2.569	63	95572	30.157	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	60.320%		
21) 2-Butanone-d5	4.624	46	90214	93.426	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	93.430%		
24) Chloroform-d	5.058	84	139243	42.722	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.440%		
26) 1,2-Dichloroethane-d4	5.698	65	92730	44.740	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.480%		
32) Benzene-d6	5.723	84	290541	42.835	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.680%		
36) 1,2-Dichloropropane-d6	6.685	67	98063	44.256	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	88.520%		
41) Toluene-d8	7.894	98	275604	43.884	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	87.760%		
43) trans-1,3-Dichloroprop...	8.173	79	46341	41.063	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	82.120%		
47) 2-Hexanone-d5	8.627	63	68926	90.048	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	90.050%		
56) 1,1,2,2-Tetrachloroeth...	10.752	84	131855	44.710	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	89.420%		
66) 1,2-Dichlorobenzene-d4	12.189	152	93066	44.514	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	89.020%		
Target Compounds						
					Qvalue	
33) Benzene	5.772	78	25773	3.854	ug/L	100
51) Chlorobenzene	9.443	112	119887	27.203	ug/L	100
64) 1,3-Dichlorobenzene	11.742	146	4858	1.580	ug/L	96
65) 1,4-Dichlorobenzene	11.832	146	40545	12.998	ug/L	99
67) 1,2-Dichlorobenzene	12.209	146	49370	15.887	ug/L	99
70) 1,2,4-trichlorobenzene	13.839	180	5722	2.901	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
Data File : VU053182.D
Acq On : 02 Mar 2023 13:02
Operator : JC/MD
Sample : 01745-05DL 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COLF2DL

Quant Time: Mar 03 01:46:24 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 03 01:44:16 2023
Response via : Initial Calibration




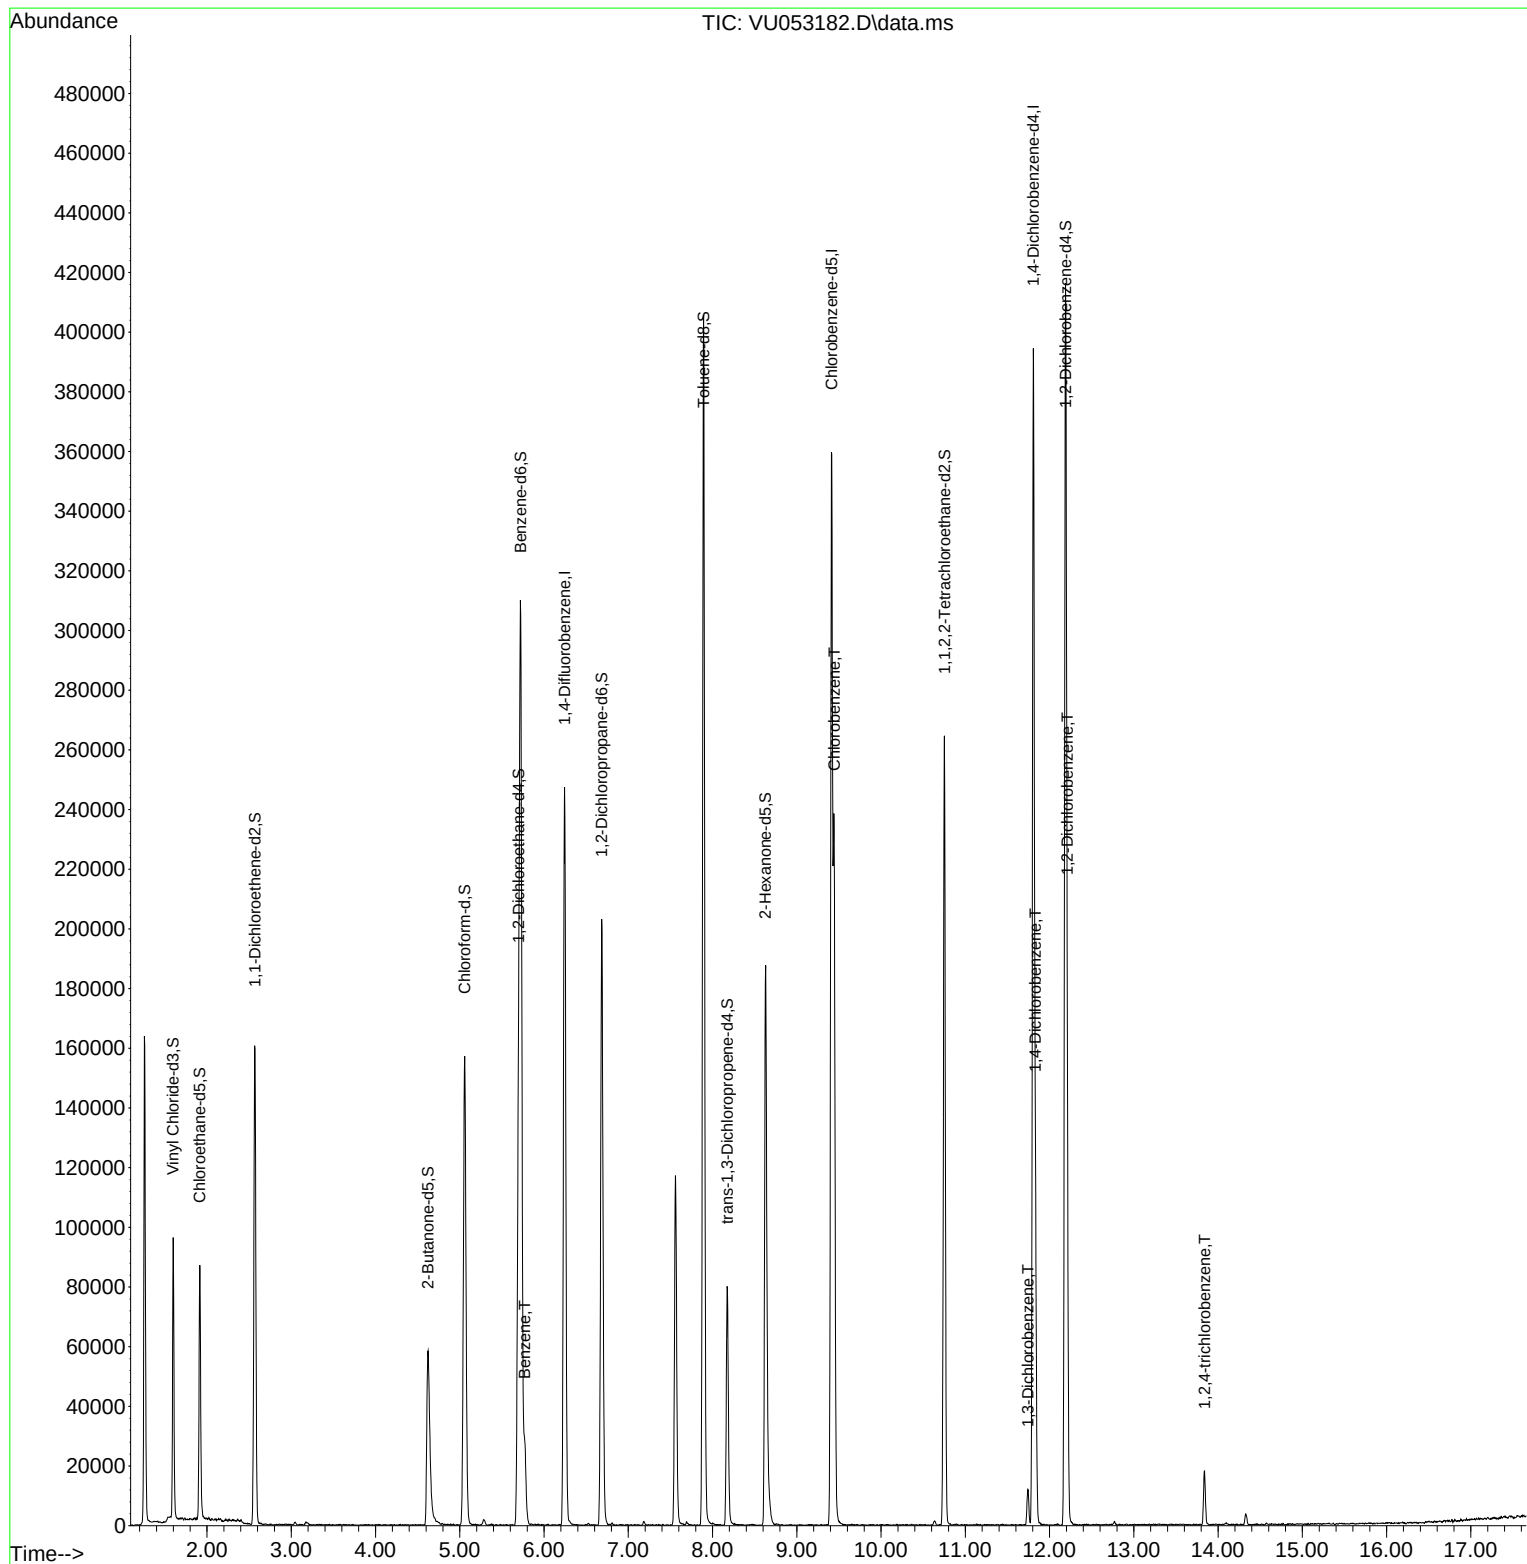


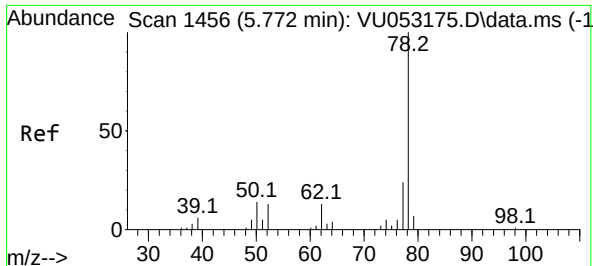

#33
Benzene
Concen: 3.854 ug/L
RT: 5.772 min Scan# 1456
Delta R.T. -0.000 min
Lab File: VU053182.D
Acq: 02 Mar 2023 13:02




Instrument :
MSVOA_U
ClientSampleId :
COLF2DL


Tgt Ion: 78 Resp: 25773

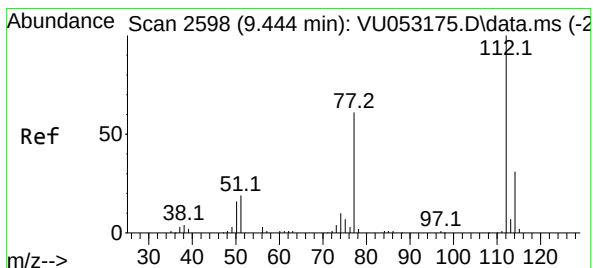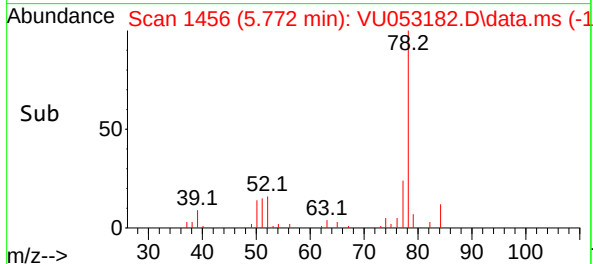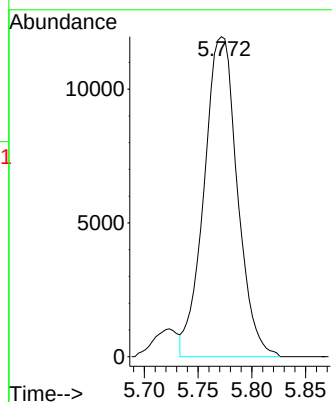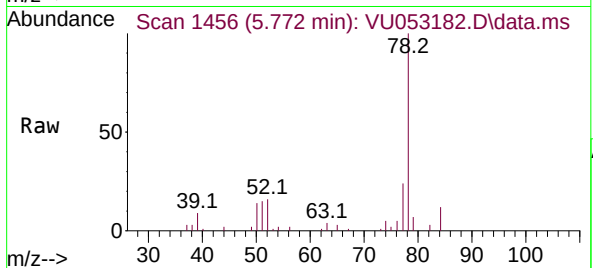

#51
Chlorobenzene
Concen: 27.203 ug/L
RT: 9.443 min Scan# 2598
Delta R.T. -0.000 min
Lab File: VU053182.D
Acq: 02 Mar 2023 13:02

Tgt Ion: 112 Resp: 119887
Ion Ratio Lower Upper
112 100
114 31.9 22.3 41.3
77 60.7 48.8 73.2

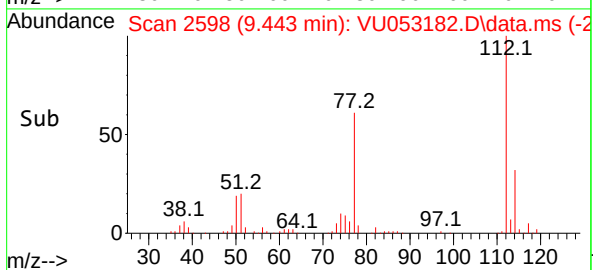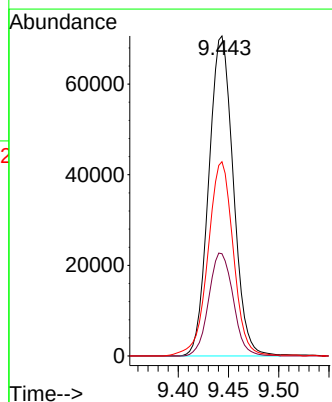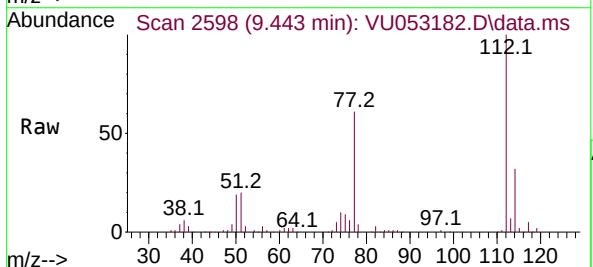

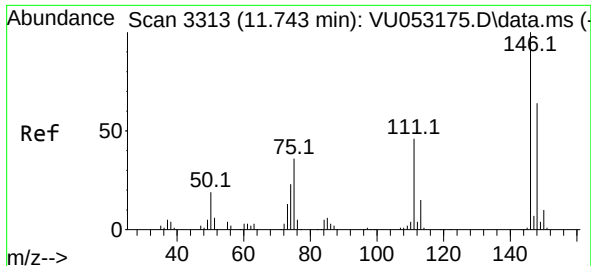

#64

1,3-Dichlorobenzene

Concen: 1.580 ug/L

RT: 11.742 min Scan# 3313

Delta R.T. -0.000 min

Lab File: VU053182.D

Acq: 02 Mar 2023 13:02

Instrument :

MSVOA_U

ClientSampleId :

C0LF2DL





Tgt Ion:146 Resp: 4858

Ion Ratio Lower Upper

146 100

111 43.3 32.1 59.5

148 60.0 44.2 82.2

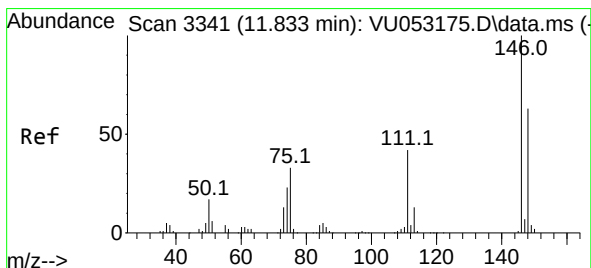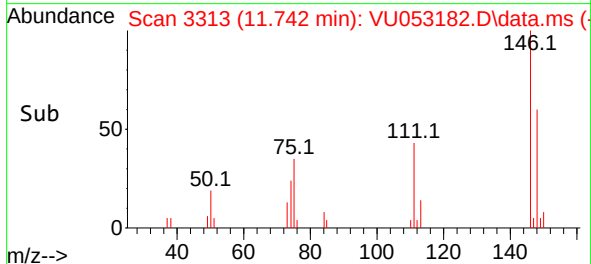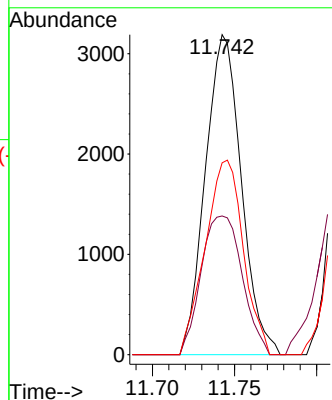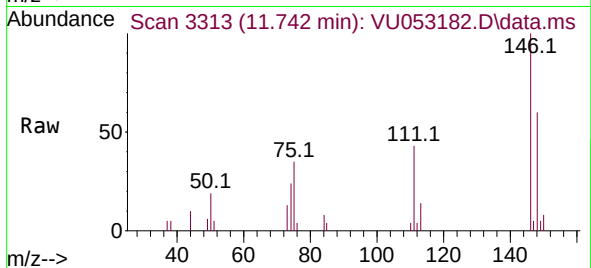

#65

1,4-Dichlorobenzene

Concen: 12.998 ug/L

RT: 11.832 min Scan# 3341

Delta R.T. -0.000 min

Lab File: VU053182.D

Acq: 02 Mar 2023 13:02




Tgt Ion:146 Resp: 40545


Ion Ratio Lower Upper

146 100

111 42.8 29.9 55.5

148 63.5 44.0 81.6

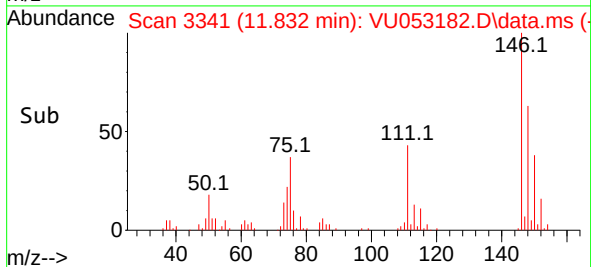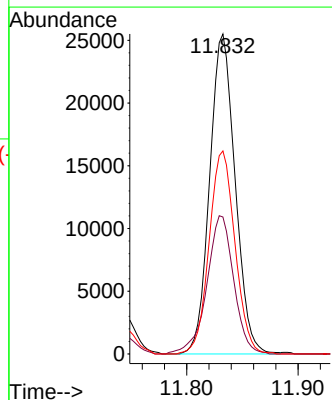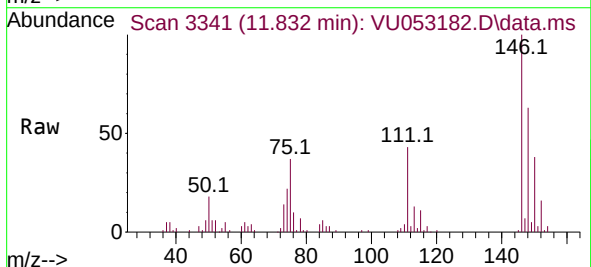

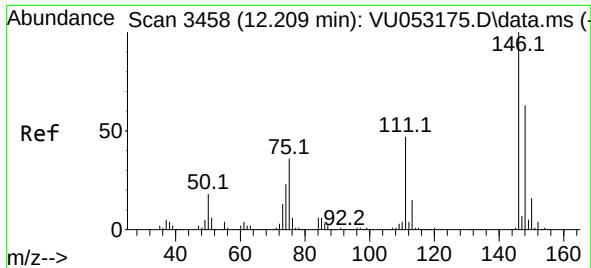

#67

1,2-Dichlorobenzene

Concen: 15.887 ug/L

RT: 12.209 min Scan# 3458

Delta R.T. -0.000 min

Lab File: VU053182.D

Acq: 02 Mar 2023 13:02

Instrument :

MSVOA_U

ClientSampleId :

COLF2DL





Tgt Ion:146 Resp: 49370

Ion Ratio Lower Upper

146 100

111 46.3 37.8 56.6

148 63.8 50.4 75.6

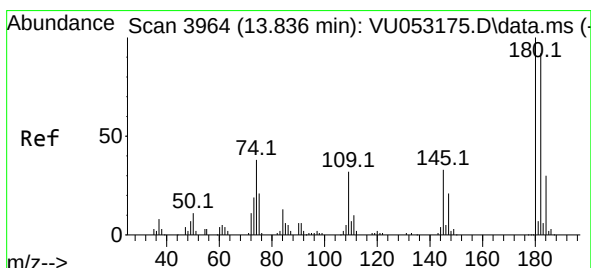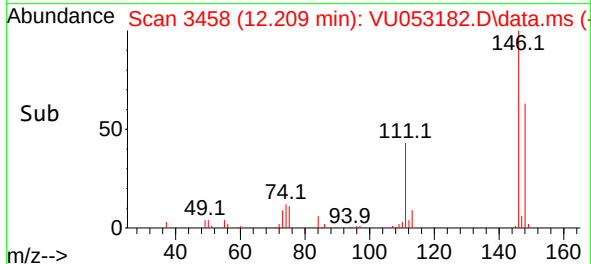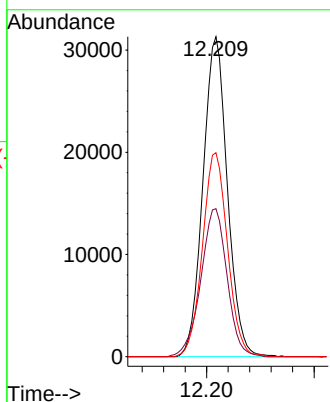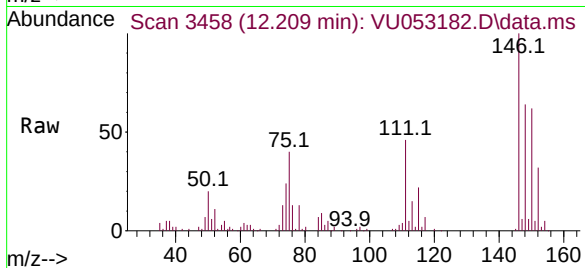

#70

1,2,4-trichlorobenzene

Concen: 2.901 ug/L

RT: 13.839 min Scan# 3965

Delta R.T. 0.003 min

Lab File: VU053182.D

Acq: 02 Mar 2023 13:02

Tgt Ion:180 Resp: 5722

Ion Ratio Lower Upper

180 100

182 88.4 76.4 114.6

145 29.5 26.8 40.2

