

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
 Data File : VU053176.D
 Acq On : 02 Mar 2023 10:28
 Operator : JC/MD
 Sample : VU0302WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK048

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
 Title : VOC Analysis

Signal : TIC: VU053176.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.141	12	16	18	rBV	276	211	0.02%	0.003%
2	1.199	29	34	35	rBV2	206	172	0.02%	0.003%
3	1.260	44	53	69	rBV	174245	225005	25.15%	3.381%
4	1.598	151	158	176	rVB	103058	117807	13.17%	1.770%
5	1.916	249	257	275	rVB	89502	119691	13.38%	1.798%
6	2.566	448	459	474	rBV	171608	278771	31.16%	4.189%
7	3.045	603	608	611	rBV3	895	949	0.11%	0.014%
8	3.858	856	861	867	rBV2	230	299	0.03%	0.004%
9	3.968	894	895	897	rVB	119	45	0.01%	0.001%
10	4.016	907	910	918	rVB	271	211	0.02%	0.003%
11	4.186	960	963	966	rBV	190	153	0.02%	0.002%
12	4.264	983	987	989	rBV	267	173	0.02%	0.003%
13	4.460	1040	1048	1050	rBV2	234	316	0.04%	0.005%
14	4.624	1087	1099	1134	rBV	58361	154755	17.30%	2.325%
15	5.000	1213	1216	1218	rVB	192	83	0.01%	0.001%
16	5.058	1218	1234	1255	rBV	167595	363157	40.60%	5.456%
17	5.206	1278	1280	1283	rVB	286	148	0.02%	0.002%
18	5.286	1295	1305	1317	rVB3	2404	4984	0.56%	0.075%
19	5.334	1317	1320	1321	rBV3	165	76	0.01%	0.001%
20	5.363	1326	1329	1332	rBV2	367	331	0.04%	0.005%
21	5.453	1355	1357	1360	rBV2	240	137	0.02%	0.002%
22	5.524	1377	1379	1382	rBV	162	92	0.01%	0.001%
23	5.591	1396	1400	1404	rBV2	173	199	0.02%	0.003%
24	5.720	1418	1440	1471	rBV2	325894	894542	100.00%	13.440%
25	6.067	1544	1548	1551	rBV	377	234	0.03%	0.004%
26	6.083	1551	1553	1558	rVB2	220	149	0.02%	0.002%
27	6.119	1559	1564	1571	rVB3	304	319	0.04%	0.005%
28	6.151	1571	1574	1575	rBV3	202	97	0.01%	0.001%
29	6.244	1590	1603	1628	rBV	237837	444333	49.67%	6.676%
30	6.427	1656	1660	1661	rBV	158	133	0.01%	0.002%
31	6.479	1674	1676	1682	rBV	256	236	0.03%	0.004%
32	6.505	1682	1684	1686	rVV	211	129	0.01%	0.002%
33	6.521	1686	1689	1698	rVB4	891	1187	0.13%	0.018%
34	6.624	1718	1721	1724	rBV	168	135	0.02%	0.002%
35	6.685	1726	1740	1762	rVV	209034	409049	45.73%	6.146%
36	6.881	1799	1801	1804	rVB2	187	108	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
 Data File : VU053176.D
 Acq On : 02 Mar 2023 10:28
 Operator : JC/MD
 Sample : VU0302WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK048

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
 Title : VOC Analysis

37	6.903	1804	1808	1810	rBV2	288	214	0.02%	0.003%
38	7.186	1888	1896	1903	rBV5	1277	1856	0.21%	0.028%
39	7.315	1934	1936	1940	rVB	246	116	0.01%	0.002%
40	7.559	2000	2012	2035	rBV	123905	219284	24.51%	3.295%
41	7.662	2042	2044	2046	rVB2	285	96	0.01%	0.001%
42	7.678	2047	2049	2051	rBV2	397	254	0.03%	0.004%
43	7.771	2075	2078	2081	rBV	222	142	0.02%	0.002%
44	7.794	2081	2085	2087	rBV2	580	405	0.05%	0.006%
45	7.832	2096	2097	2099	rBV2	122	54	0.01%	0.001%
46	7.894	2103	2116	2138	rVV	424812	731113	81.73%	10.985%
47	8.173	2192	2203	2228	rBV	84606	145605	16.28%	2.188%
48	8.308	2241	2245	2247	rBV2	424	229	0.03%	0.003%
49	8.353	2257	2259	2263	rBV2	247	219	0.02%	0.003%
50	8.530	2312	2314	2316	rBV	151	41	0.00%	0.001%
51	8.630	2333	2345	2379	rBV2	189335	363068	40.59%	5.455%
52	8.842	2405	2411	2412	rBB	29	102	0.01%	0.002%
53	9.035	2468	2471	2473	rBV	188	93	0.01%	0.001%
54	9.160	2507	2510	2515	rVB2	305	300	0.03%	0.005%
55	9.411	2576	2588	2614	rBV	331973	551816	61.69%	8.291%
56	9.668	2665	2668	2671	rBV2	269	235	0.03%	0.004%
57	9.730	2683	2687	2689	rBV2	203	186	0.02%	0.003%
58	9.958	2754	2758	2762	rBV2	310	291	0.03%	0.004%
59	10.096	2798	2801	2802	rBV	328	172	0.02%	0.003%
60	10.186	2827	2829	2832	rBV	156	113	0.01%	0.002%
61	10.411	2897	2899	2903	rBV2	157	144	0.02%	0.002%
62	10.633	2960	2968	2977	rVB2	3926	5744	0.64%	0.086%
63	10.752	2992	3005	3023	rBV	266883	429239	47.98%	6.449%
64	10.839	3029	3032	3035	rVB2	364	198	0.02%	0.003%
65	10.900	3048	3051	3055	rBV	193	138	0.02%	0.002%
66	11.228	3150	3153	3158	rBV2	226	242	0.03%	0.004%
67	11.463	3222	3226	3227	rBV2	711	541	0.06%	0.008%
68	11.662	3285	3288	3292	rBV	200	153	0.02%	0.002%
69	11.681	3292	3294	3298	rVV2	247	165	0.02%	0.002%
70	11.807	3321	3333	3356	rBV	348103	551307	61.63%	8.283%
71	12.189	3439	3452	3470	rBV	373440	611629	68.37%	9.190%
72	12.379	3508	3511	3514	rBV	274	190	0.02%	0.003%
73	12.752	3623	3627	3628	rBV2	291	186	0.02%	0.003%
74	12.794	3638	3640	3648	rVB	187	156	0.02%	0.002%
75	13.218	3768	3772	3773	rBV2	800	583	0.07%	0.009%
76	13.845	3960	3967	3974	rBV5	3205	4338	0.48%	0.065%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
Data File : VU053176.D
Acq On : 02 Mar 2023 10:28
Operator : JC/MD
Sample : VU0302WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK048

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Title : VOC Analysis

77	14.044	4026	4029	4031	rBV2	202	134	0.01%	0.002%
78	14.089	4032	4043	4053	rBV	6394	10161	1.14%	0.153%
79	14.331	4111	4118	4131	rVB6	3625	5717	0.64%	0.086%
80	14.729	4240	4242	4245	rBV	294	195	0.02%	0.003%


Sum of corrected areas: 6655580

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
Data File : VU053176.D
Acq On : 02 Mar 2023 10:28
Operator : JC/MD
Sample : VU0302WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK048

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

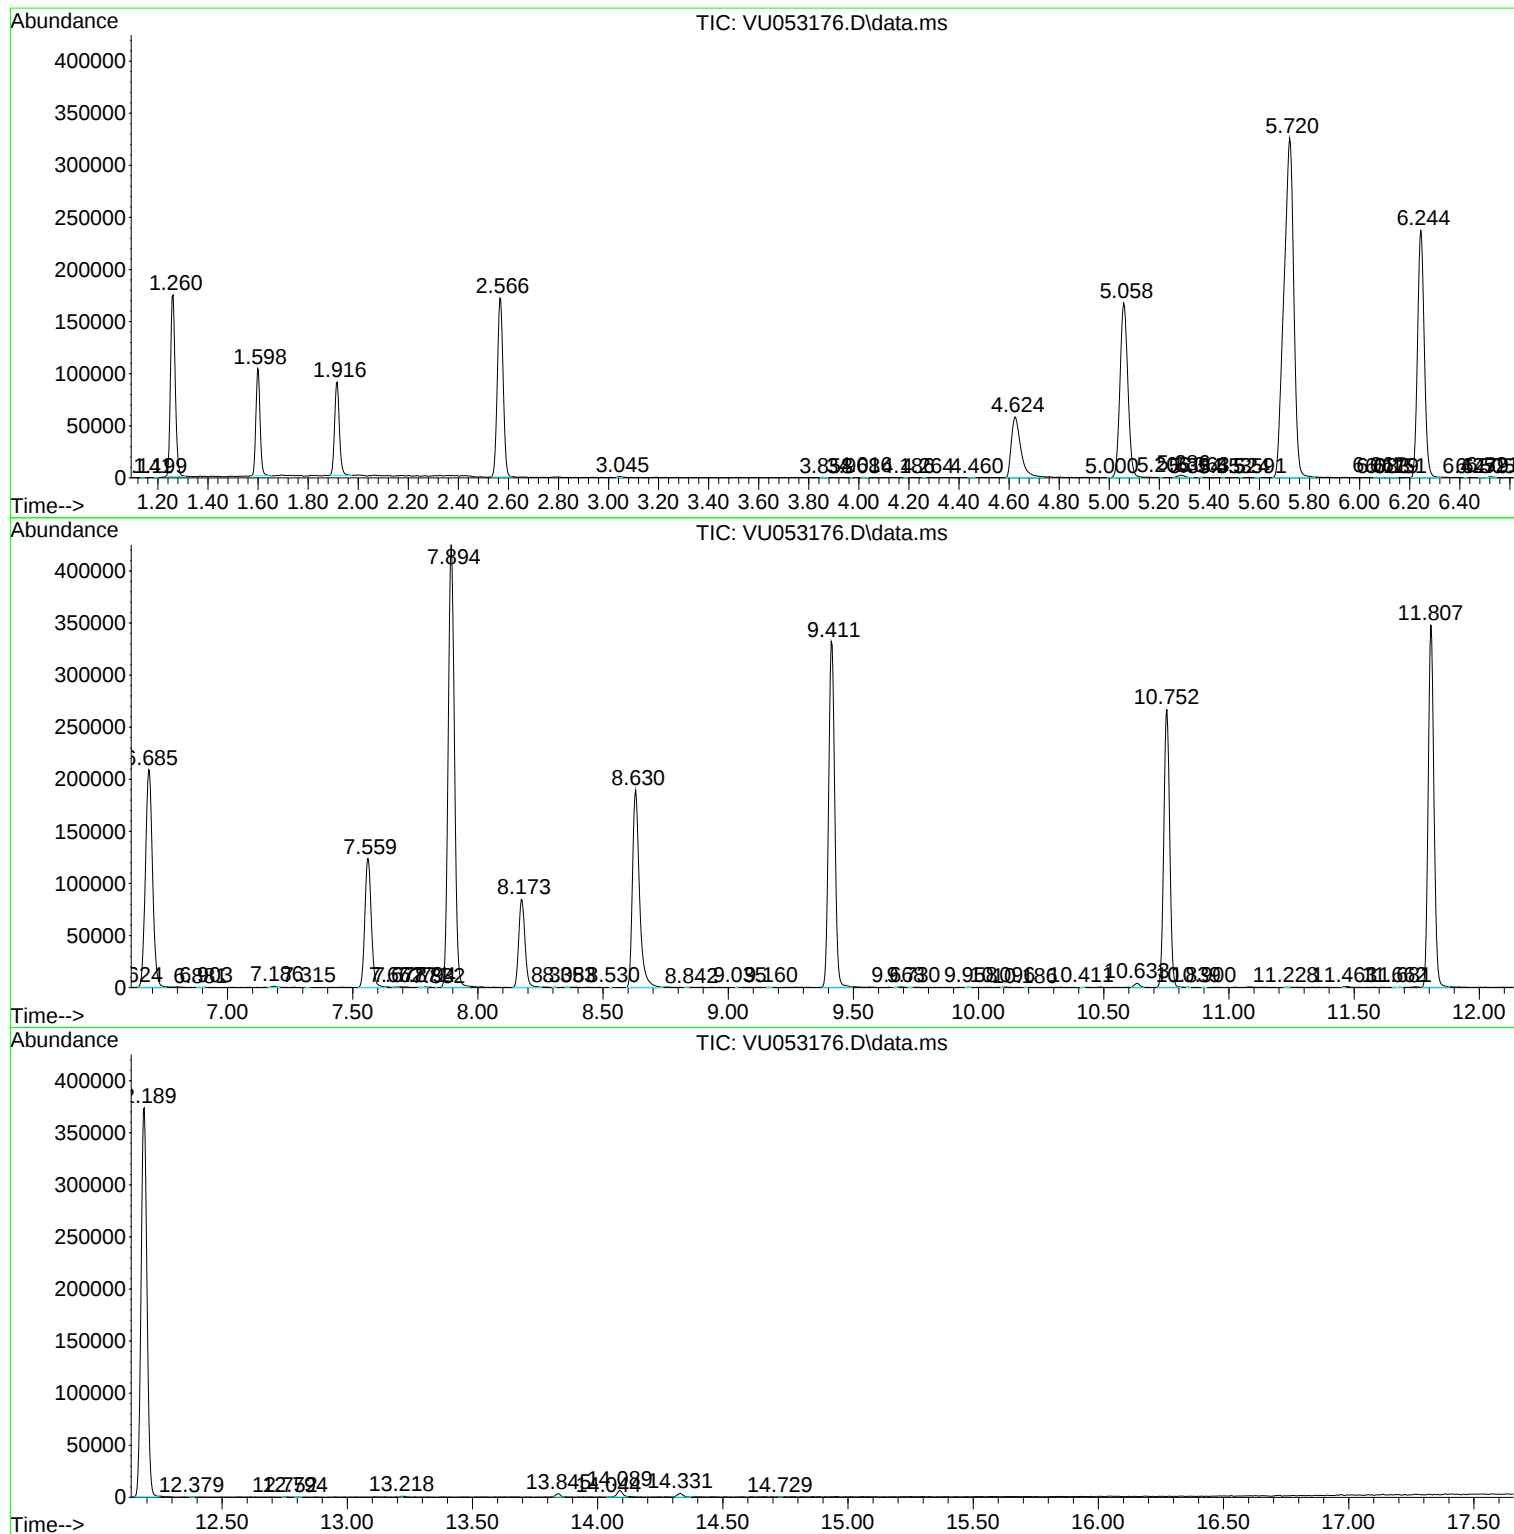

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
Data File : VU053176.D
Acq On : 02 Mar 2023 10:28
Operator : JC/MD
Sample : VU0302WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK048

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
Data File : VU053176.D
Acq On : 02 Mar 2023 10:28
Operator : JC/MD
Sample : VU0302WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK048

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------