

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
 Data File : VU053178.D
 Acq On : 02 Mar 2023 11:28
 Operator : JC/MD
 Sample : 01745-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLE9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
 Title : VOC Analysis

Signal : TIC: VU053178.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.135	11	14	18	rVB	187	116	0.01%	0.002%
2	1.154	18	20	22	rBV	151	87	0.01%	0.002%
3	1.170	22	25	33	rVB2	242	265	0.03%	0.005%
4	1.257	33	52	64	rBV	69731	87993	11.35%	1.623%
5	1.598	152	158	173	rVB	89096	103069	13.30%	1.901%
6	1.913	249	256	268	rBV	77933	102725	13.26%	1.894%
7	2.566	447	459	475	rBV	147937	242109	31.24%	4.465%
8	3.183	640	651	664	rVB2	5263	11149	1.44%	0.206%
9	3.489	744	746	748	rBV	189	113	0.01%	0.002%
10	3.569	768	771	773	rBV	159	96	0.01%	0.002%
11	3.971	892	896	898	rBV	355	313	0.04%	0.006%
12	4.106	935	938	940	rBV	324	257	0.03%	0.005%
13	4.405	1029	1031	1032	rBV	169	60	0.01%	0.001%
14	4.624	1087	1099	1132	rBV2	59405	162560	20.98%	2.998%
15	5.058	1219	1234	1264	rVB	143415	316541	40.84%	5.838%
16	5.276	1293	1302	1303	rBV4	1670	1566	0.20%	0.029%
17	5.370	1326	1331	1338	rVB4	502	692	0.09%	0.013%
18	5.498	1369	1371	1372	rBV4	145	61	0.01%	0.001%
19	5.537	1381	1383	1386	rVB	162	53	0.01%	0.001%
20	5.592	1397	1400	1402	rVB	185	89	0.01%	0.002%
21	5.720	1420	1440	1461	rBV2	283101	774987	100.00%	14.293%
22	5.910	1496	1499	1501	rBV2	229	141	0.02%	0.003%
23	5.926	1501	1504	1509	rVB2	220	159	0.02%	0.003%
24	5.971	1516	1518	1521	rBV	156	70	0.01%	0.001%
25	6.019	1531	1533	1538	rVB	257	172	0.02%	0.003%
26	6.193	1585	1587	1588	rBV	128	56	0.01%	0.001%
27	6.244	1589	1603	1629	rVV	156255	294991	38.06%	5.440%
28	6.508	1682	1685	1693	rBV2	252	356	0.05%	0.007%
29	6.550	1696	1698	1701	rBV2	150	88	0.01%	0.002%
30	6.685	1727	1740	1763	rBV	178502	352861	45.53%	6.508%
31	6.800	1768	1776	1785	rVB4	670	905	0.12%	0.017%
32	6.839	1785	1788	1792	rBV	197	133	0.02%	0.002%
33	6.884	1799	1802	1805	rBV	223	148	0.02%	0.003%
34	6.990	1833	1835	1838	rVB	208	95	0.01%	0.002%
35	7.009	1839	1841	1846	rBV	158	76	0.01%	0.001%
36	7.186	1891	1896	1904	rBV4	900	1148	0.15%	0.021%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
 Data File : VU053178.D
 Acq On : 02 Mar 2023 11:28
 Operator : JC/MD
 Sample : 01745-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLE9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
 Title : VOC Analysis

37	7.363	1948	1951	1954	rBV2	228	148	0.02%	0.003%
38	7.482	1987	1988	1990	rBV	124	33	0.00%	0.001%
39	7.501	1991	1994	1997	rVB	207	106	0.01%	0.002%
40	7.563	2001	2013	2032	rBV	106485	189707	24.48%	3.499%
41	7.723	2061	2063	2065	rVB	200	82	0.01%	0.002%
42	7.797	2083	2086	2087	rBV	187	102	0.01%	0.002%
43	7.894	2103	2116	2140	rBV	371215	635191	81.96%	11.714%
44	8.177	2189	2204	2224	rBV	71017	124423	16.05%	2.295%
45	8.292	2236	2240	2241	rBV2	293	205	0.03%	0.004%
46	8.334	2251	2253	2256	rVB2	242	114	0.01%	0.002%
47	8.405	2273	2275	2279	rBV2	251	181	0.02%	0.003%
48	8.630	2333	2345	2374	rBV2	157726	306144	39.50%	5.646%
49	8.842	2407	2411	2414	rBV2	312	373	0.05%	0.007%
50	8.878	2420	2422	2427	rVB2	234	189	0.02%	0.003%
51	8.897	2427	2428	2429	rBV2	120	26	0.00%	0.000%
52	8.913	2431	2433	2436	rBV	197	136	0.02%	0.003%
53	8.993	2456	2458	2461	rVB2	251	133	0.02%	0.002%
54	9.251	2536	2538	2541	rBV2	150	101	0.01%	0.002%
55	9.263	2541	2542	2543	rVB2	106	20	0.00%	0.000%
56	9.283	2544	2548	2551	rBV2	215	201	0.03%	0.004%
57	9.415	2576	2589	2613	rBV	218130	366149	47.25%	6.753%
58	9.588	2642	2643	2646	rBV	224	144	0.02%	0.003%
59	9.633	2654	2657	2661	rBV2	225	194	0.03%	0.004%
60	9.775	2699	2701	2702	rBV2	126	34	0.00%	0.001%
61	9.951	2754	2756	2758	rBV	158	64	0.01%	0.001%
62	10.164	2819	2822	2824	rBV2	195	111	0.01%	0.002%
63	10.324	2869	2872	2874	rBV	202	112	0.01%	0.002%
64	10.636	2962	2969	2976	rBV3	1750	2621	0.34%	0.048%
65	10.752	2993	3005	3024	rBV	234223	375476	48.45%	6.925%
66	10.890	3041	3048	3052	rBV2	799	1032	0.13%	0.019%
67	11.549	3250	3253	3254	rBV	224	106	0.01%	0.002%
68	11.611	3270	3272	3273	rBV	132	31	0.00%	0.001%
69	11.652	3282	3285	3287	rBV	299	217	0.03%	0.004%
70	11.807	3321	3333	3355	rBV	228885	368631	47.57%	6.798%
71	11.942	3372	3375	3380	rVB2	236	208	0.03%	0.004%
72	12.016	3396	3398	3400	rBV2	213	127	0.02%	0.002%
73	12.189	3438	3452	3474	rBV	339363	562271	72.55%	10.370%
74	12.514	3550	3553	3555	rVB	192	87	0.01%	0.002%
75	13.041	3714	3717	3721	rBV2	273	250	0.03%	0.005%
76	13.080	3727	3729	3732	rVB	222	90	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
Data File : VU053178.D
Acq On : 02 Mar 2023 11:28
Operator : JC/MD
Sample : 01745-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0LE9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Title : VOC Analysis

77	13.295	3793	3796	3799	rBV	265	177	0.02%	0.003%
78	13.839	3956	3965	3978	rBV2	8064	12680	1.64%	0.234%
79	14.086	4038	4042	4055	rVB5	1101	2009	0.26%	0.037%
80	14.328	4109	4117	4130	rVB4	7333	11057	1.43%	0.204%
81	15.080	4350	4351	4352	rBV4	221	71	0.01%	0.001%
82	15.999	4631	4637	4645	rVB5	3139	4448	0.57%	0.082%




Sum of corrected areas: 5422312

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
Data File : VU053178.D
Acq On : 02 Mar 2023 11:28
Operator : JC/MD
Sample : 01745-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COLE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

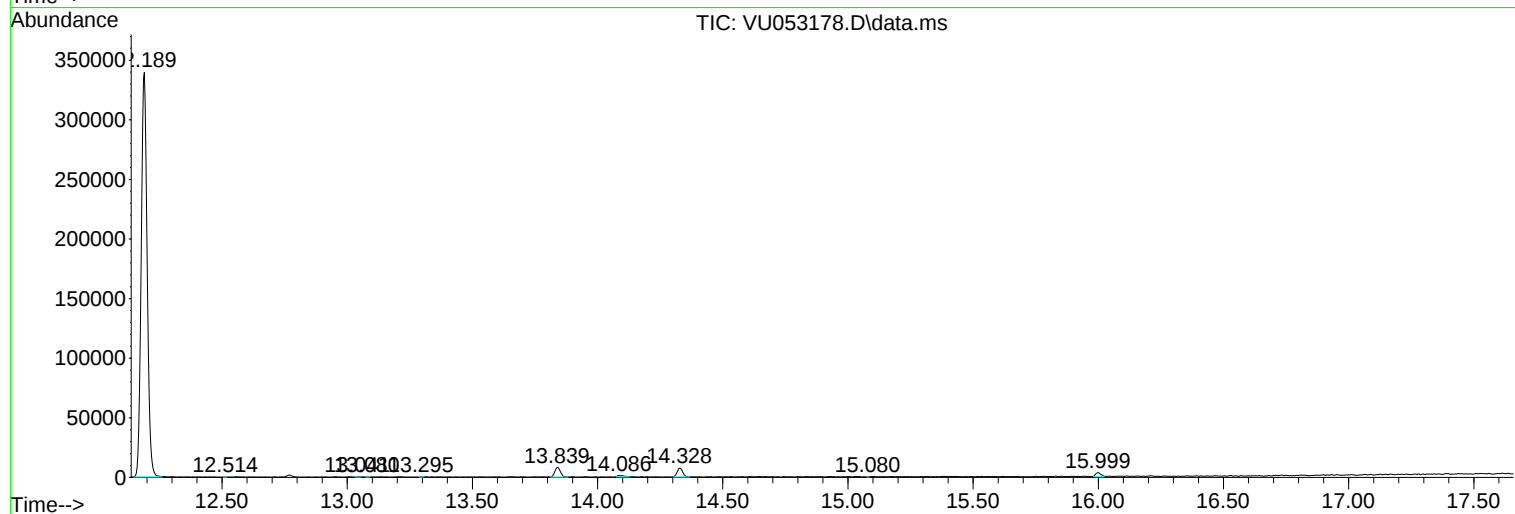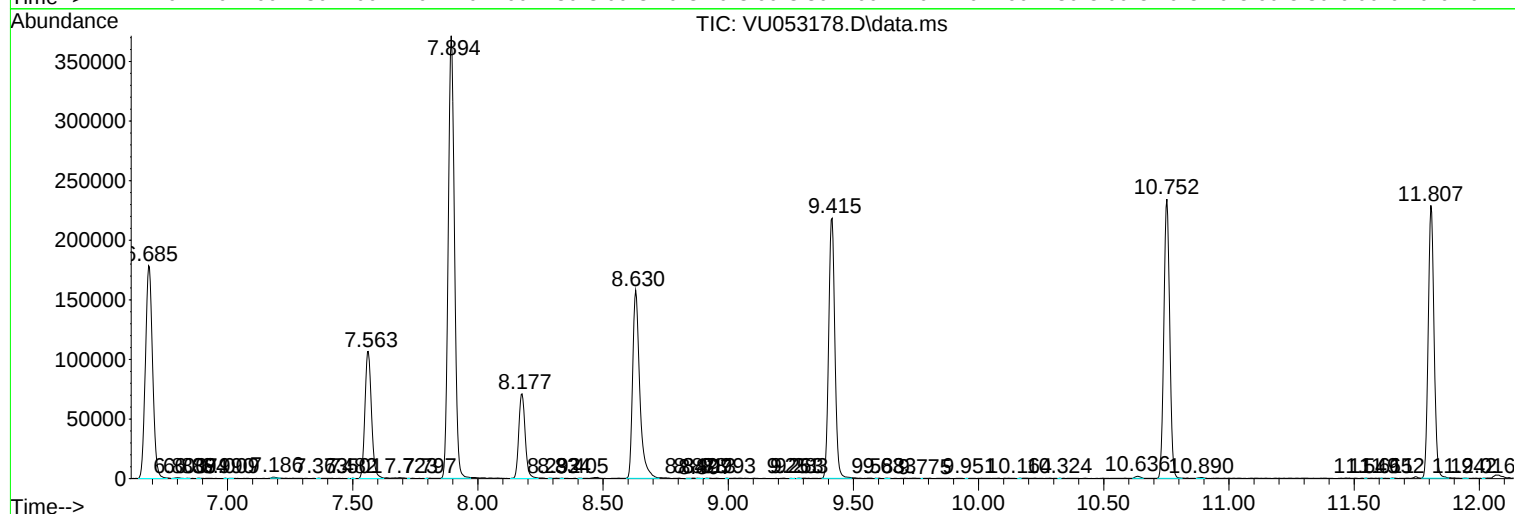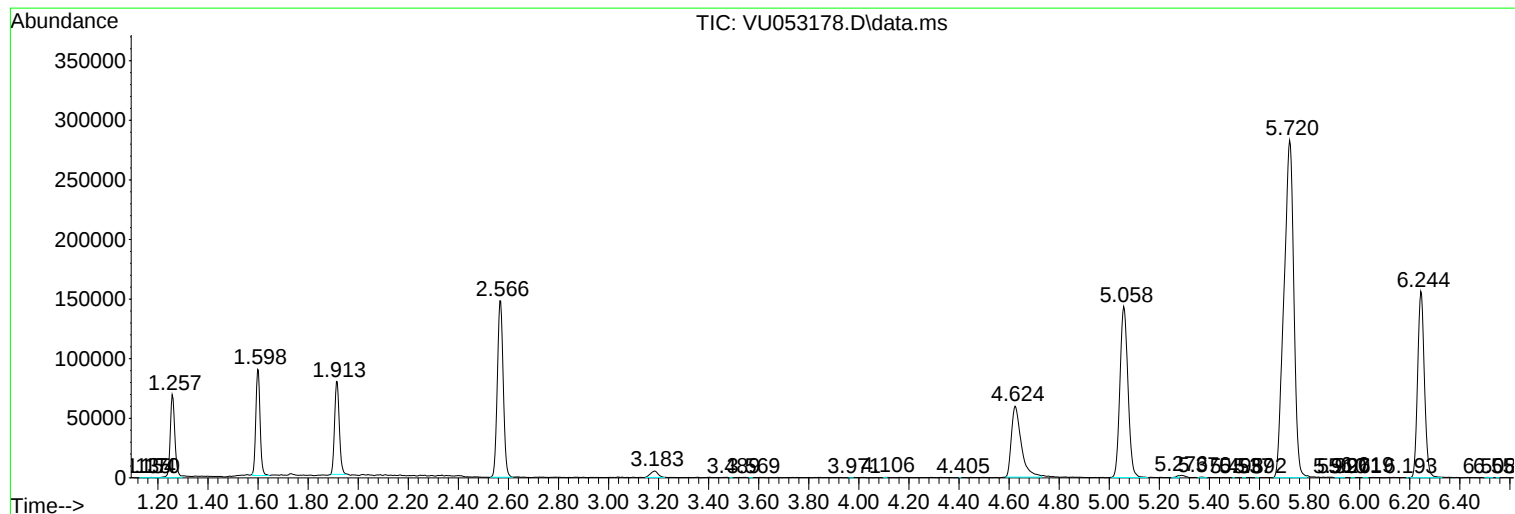

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
Data File : VU053178.D
Acq On : 02 Mar 2023 11:28
Operator : JC/MD
Sample : 01745-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0LE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
Data File : VU053178.D
Acq On : 02 Mar 2023 11:28
Operator : JC/MD
Sample : 01745-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0LE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc