

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
 Data File : VU053179.D
 Acq On : 02 Mar 2023 11:51
 Operator : JC/MD
 Sample : 01745-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLFO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
 Title : VOC Analysis

Signal : TIC: VU053179.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.135	13	14	15	rVB	116	22	0.00%	0.000%
2	1.151	15	19	23	rBV2	178	200	0.01%	0.002%
3	1.257	45	52	65	rVB	55150	65332	3.82%	0.590%
4	1.598	151	158	171	rVB	188817	218340	12.77%	1.973%
5	1.916	248	257	272	rVB	170854	229040	13.40%	2.070%
6	2.566	447	459	477	rBV	328631	530610	31.04%	4.794%
7	2.733	508	511	515	rBV2	405	362	0.02%	0.003%
8	3.183	637	651	670	rVB	9016	20536	1.20%	0.186%
9	3.566	767	770	771	rBV	193	96	0.01%	0.001%
10	3.756	826	829	832	rBV2	199	132	0.01%	0.001%
11	3.907	872	876	883	rBV2	274	359	0.02%	0.003%
12	4.019	908	911	914	rBV2	254	215	0.01%	0.002%
13	4.167	954	957	958	rBV	177	99	0.01%	0.001%
14	4.273	986	990	992	rBV	195	142	0.01%	0.001%
15	4.492	1054	1058	1059	rBV	181	116	0.01%	0.001%
16	4.620	1085	1098	1142	rBV2	122440	335832	19.64%	3.034%
17	5.058	1217	1234	1261	rBV	321915	701488	41.03%	6.338%
18	5.251	1290	1294	1295	rBV2	184	161	0.01%	0.001%
19	5.283	1295	1304	1319	rVB2	2137	4153	0.24%	0.038%
20	5.366	1327	1330	1331	rBV2	374	232	0.01%	0.002%
21	5.434	1347	1351	1354	rBV2	180	165	0.01%	0.001%
22	5.534	1379	1382	1385	rBV2	173	127	0.01%	0.001%
23	5.620	1407	1409	1411	rBV	171	88	0.01%	0.001%
24	5.720	1419	1440	1471	rBV2	630140	1709606	100.00%	15.447%
25	6.109	1560	1561	1562	rBV2	187	60	0.00%	0.001%
26	6.141	1569	1571	1572	rBV	205	82	0.00%	0.001%
27	6.177	1581	1582	1586	rBV	127	62	0.00%	0.001%
28	6.244	1590	1603	1627	rBV	234118	438970	25.68%	3.966%
29	6.501	1681	1683	1685	rBV	168	87	0.01%	0.001%
30	6.553	1697	1699	1700	rBV	167	90	0.01%	0.001%
31	6.607	1711	1716	1722	rVB2	352	528	0.03%	0.005%
32	6.685	1722	1740	1762	rBV	401885	789751	46.19%	7.136%
33	6.865	1794	1796	1800	rVB	239	139	0.01%	0.001%
34	7.013	1839	1842	1846	rBV2	228	169	0.01%	0.002%
35	7.103	1868	1870	1873	rVB	181	121	0.01%	0.001%
36	7.122	1873	1876	1878	rBV	119	76	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
 Data File : VU053179.D
 Acq On : 02 Mar 2023 11:51
 Operator : JC/MD
 Sample : 01745-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLFO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
 Title : VOC Analysis

37	7.183	1886	1895	1905	rBV3	2643	4957	0.29%	0.045%
38	7.424	1966	1970	1972	rBV	224	176	0.01%	0.002%
39	7.460	1978	1981	1986	rBV2	159	165	0.01%	0.001%
40	7.559	1999	2012	2037	rBV	245142	432408	25.29%	3.907%
41	7.688	2045	2052	2061	rVB5	1644	2796	0.16%	0.025%
42	7.768	2075	2077	2078	rBV5	119	50	0.00%	0.000%
43	7.791	2082	2084	2087	rVB2	306	148	0.01%	0.001%
44	7.894	2101	2116	2133	rBV	821251	1401136	81.96%	12.660%
45	8.090	2174	2177	2184	rVB2	364	302	0.02%	0.003%
46	8.128	2184	2189	2192	rBV2	237	223	0.01%	0.002%
47	8.173	2192	2203	2231	rBV	168193	285602	16.71%	2.581%
48	8.382	2264	2268	2270	rBV	163	128	0.01%	0.001%
49	8.398	2270	2273	2276	rVV2	283	197	0.01%	0.002%
50	8.431	2280	2283	2286	rBV	149	94	0.01%	0.001%
51	8.630	2333	2345	2382	rBV2	375299	707255	41.37%	6.391%
52	8.816	2401	2403	2405	rBV	280	151	0.01%	0.001%
53	8.858	2414	2416	2417	rBV	177	56	0.00%	0.001%
54	8.955	2444	2446	2449	rVB	180	83	0.00%	0.001%
55	8.974	2449	2452	2456	rBV2	258	198	0.01%	0.002%
56	9.022	2463	2467	2469	rBV2	211	157	0.01%	0.001%
57	9.135	2496	2502	2506	rBV	323	475	0.03%	0.004%
58	9.157	2507	2509	2511	rBV2	238	139	0.01%	0.001%
59	9.225	2528	2530	2533	rVB	162	50	0.00%	0.000%
60	9.289	2547	2550	2555	rBV2	179	135	0.01%	0.001%
61	9.337	2563	2565	2568	rBV	152	69	0.00%	0.001%
62	9.411	2576	2588	2612	rBV	320236	538577	31.50%	4.866%
63	9.569	2633	2637	2639	rBV2	241	154	0.01%	0.001%
64	10.070	2791	2793	2800	rVB2	288	218	0.01%	0.002%
65	10.160	2818	2821	2826	rBV	252	205	0.01%	0.002%
66	10.466	2914	2916	2919	rBV	143	37	0.00%	0.000%
67	10.601	2955	2958	2961	rBV2	275	232	0.01%	0.002%
68	10.633	2962	2968	2978	rVB3	1578	2422	0.14%	0.022%
69	10.749	2991	3004	3023	rBV	529643	840107	49.14%	7.591%
70	10.887	3042	3047	3055	rVB3	947	995	0.06%	0.009%
71	10.948	3064	3066	3068	rBV	138	48	0.00%	0.000%
72	10.974	3072	3074	3078	rBV	171	141	0.01%	0.001%
73	11.041	3091	3095	3100	rBV	298	286	0.02%	0.003%
74	11.135	3116	3124	3127	rBV3	467	688	0.04%	0.006%
75	11.270	3162	3166	3170	rBV2	169	120	0.01%	0.001%
76	11.405	3206	3208	3209	rVB2	200	52	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
 Data File : VU053179.D
 Acq On : 02 Mar 2023 11:51
 Operator : JC/MD
 Sample : 01745-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLFO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M

Title : VOC Analysis

77	11.440	3215	3219	3222	rBV2	260	179	0.01%	0.002%
78	11.463	3225	3226	3230	rBV	254	185	0.01%	0.002%
79	11.697	3296	3299	3302	rBV2	273	215	0.01%	0.002%
80	11.807	3321	3333	3355	rBV	354336	557755	32.62%	5.040%
81	12.186	3438	3451	3469	rBV	766287	1231977	72.06%	11.132%
82	12.311	3487	3490	3498	rVB2	450	390	0.02%	0.004%
83	12.765	3624	3631	3633	rBV2	1111	1375	0.08%	0.012%
84	13.839	3961	3965	3973	rVB4	2621	3249	0.19%	0.029%
85	14.324	4110	4116	4126	rVB5	2065	2888	0.17%	0.026%




Sum of corrected areas: 11067233

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
Data File : VU053179.D
Acq On : 02 Mar 2023 11:51
Operator : JC/MD
Sample : 01745-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COLFO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

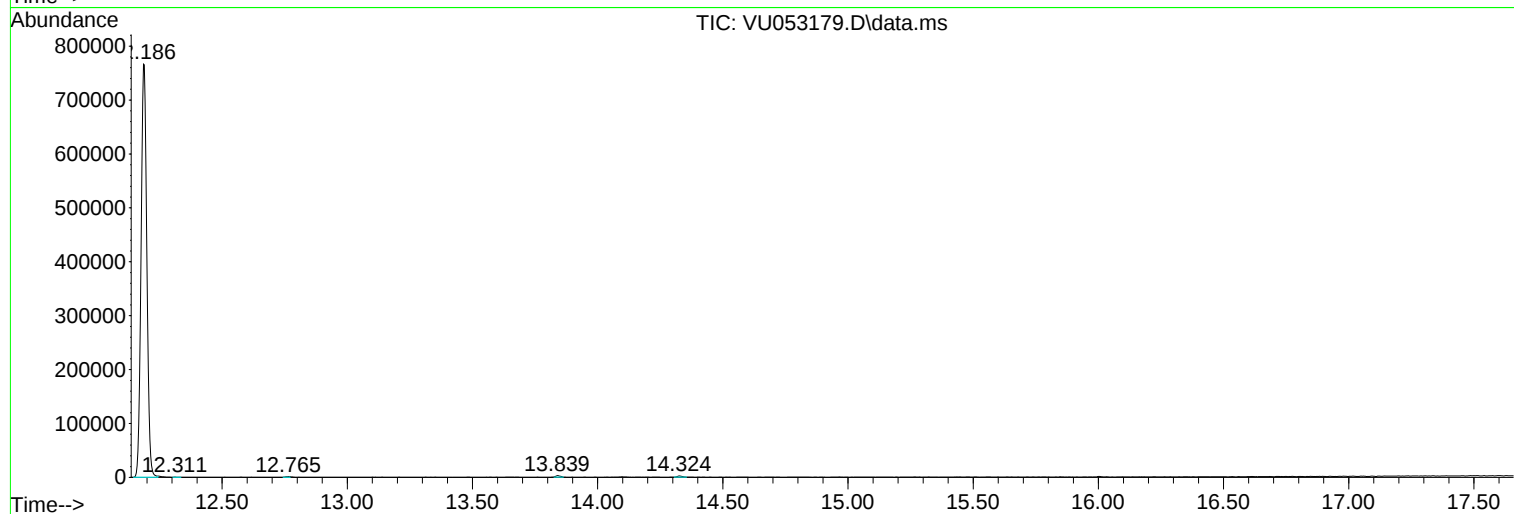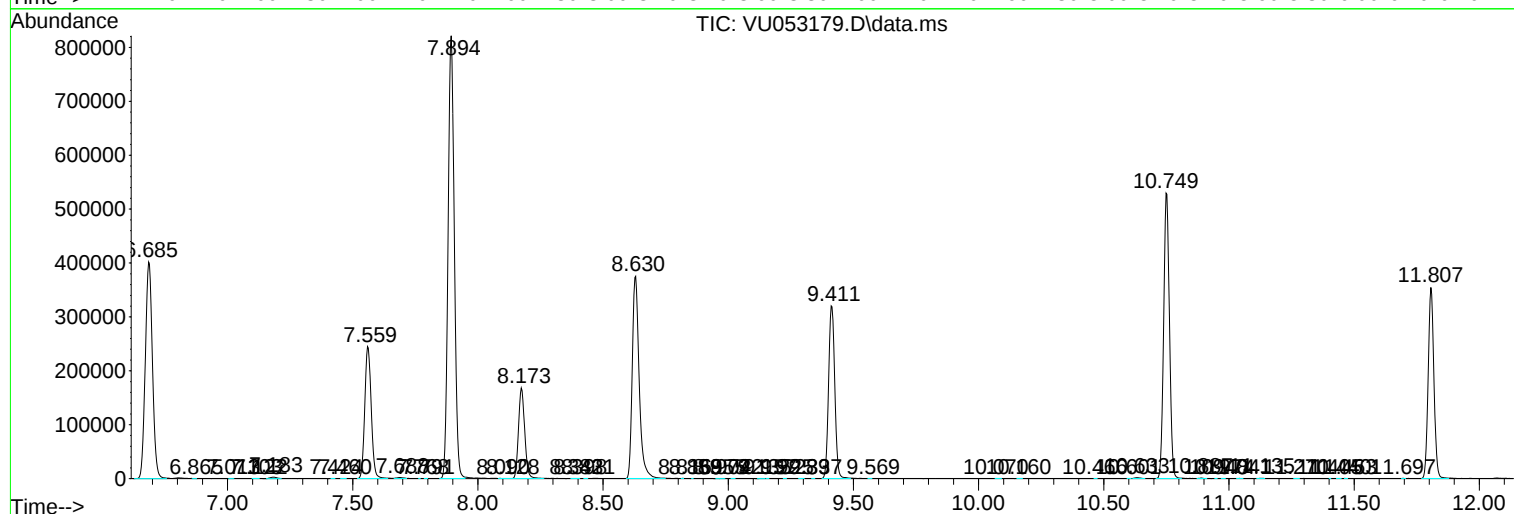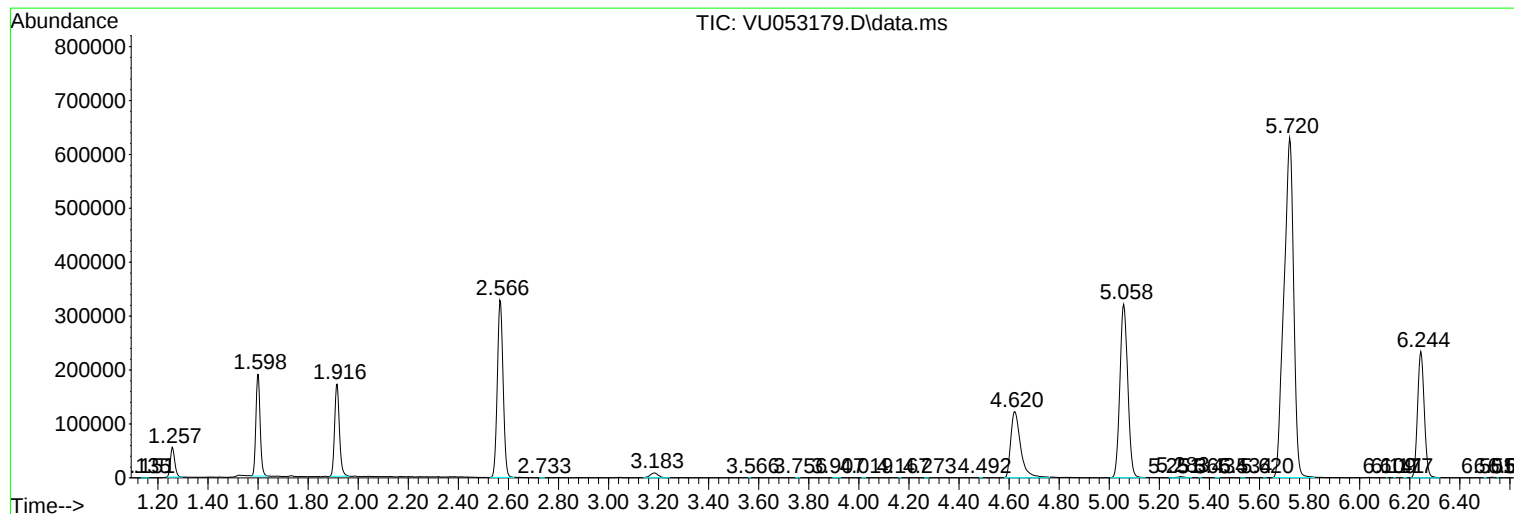

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
Data File : VU053179.D
Acq On : 02 Mar 2023 11:51
Operator : JC/MD
Sample : 01745-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COLFO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
Data File : VU053179.D
Acq On : 02 Mar 2023 11:51
Operator : JC/MD
Sample : 01745-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COLFO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc