

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
 Data File : VU053180.D
 Acq On : 02 Mar 2023 12:15
 Operator : JC/MD
 Sample : 01745-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M

Title : VOC Analysis

Signal : TIC: VU053180.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.193	25	32	35	rBV	302	371	0.04%	0.006%
2	1.257	45	52	64	rBV	61124	71748	8.29%	1.094%
3	1.598	152	158	172	rVB	96012	112034	12.95%	1.709%
4	1.913	248	256	274	rVB	86892	116643	13.48%	1.779%
5	2.566	447	459	474	rBV	163842	269309	31.12%	4.108%
6	2.794	528	530	534	rBV	320	260	0.03%	0.004%
7	3.180	641	650	666	rVB	7185	16084	1.86%	0.245%
8	3.421	718	725	731	rBB2	263	336	0.04%	0.005%
9	3.450	732	734	739	rVB2	239	182	0.02%	0.003%
10	3.640	790	793	799	rVB2	240	233	0.03%	0.004%
11	3.675	799	804	810	rVB2	268	319	0.04%	0.005%
12	3.887	866	870	873	rBV2	174	183	0.02%	0.003%
13	4.344	1009	1012	1017	rBV	334	312	0.04%	0.005%
14	4.450	1042	1045	1049	rBV	292	209	0.02%	0.003%
15	4.505	1059	1062	1067	rBV2	190	179	0.02%	0.003%
16	4.543	1071	1074	1077	rBV	250	185	0.02%	0.003%
17	4.624	1081	1099	1134	rBV3	67821	190030	21.96%	2.899%
18	5.058	1218	1234	1257	rBV	160845	354082	40.92%	5.401%
19	5.202	1275	1279	1284	rVB2	274	215	0.02%	0.003%
20	5.228	1284	1287	1291	rVB	251	192	0.02%	0.003%
21	5.254	1291	1295	1297	rBV	256	155	0.02%	0.002%
22	5.286	1297	1305	1318	rVV2	1792	3119	0.36%	0.048%
23	5.341	1318	1322	1326	rVB2	217	240	0.03%	0.004%
24	5.607	1403	1405	1410	rBV2	197	216	0.02%	0.003%
25	5.720	1419	1440	1469	rBV2	322502	865335	100.00%	13.200%
26	5.935	1504	1507	1514	rVB2	371	361	0.04%	0.006%
27	5.971	1514	1518	1519	rBV	296	150	0.02%	0.002%
28	6.045	1538	1541	1544	rBV2	292	207	0.02%	0.003%
29	6.077	1549	1551	1556	rVB	212	180	0.02%	0.003%
30	6.244	1588	1603	1623	rBV	248196	470292	54.35%	7.174%
31	6.389	1646	1648	1652	rVB2	278	163	0.02%	0.002%
32	6.418	1654	1657	1664	rVB3	260	236	0.03%	0.004%
33	6.450	1664	1667	1670	rBV	214	153	0.02%	0.002%
34	6.524	1686	1690	1693	rBV3	307	246	0.03%	0.004%
35	6.685	1725	1740	1764	rBV	207431	399790	46.20%	6.099%
36	6.948	1817	1822	1826	rBV2	221	250	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
 Data File : VU053180.D
 Acq On : 02 Mar 2023 12:15
 Operator : JC/MD
 Sample : 01745-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
 Title : VOC Analysis

37	7.186	1890	1896	1904	rBV3	1072	1638	0.19%	0.025%
38	7.289	1925	1928	1931	rBV2	194	163	0.02%	0.002%
39	7.562	2000	2013	2032	rBV	122519	213780	24.70%	3.261%
40	7.652	2038	2041	2043	rBV2	267	169	0.02%	0.003%
41	7.894	2099	2116	2142	rBV	408880	706777	81.68%	10.782%
42	8.087	2174	2176	2181	rBV2	291	233	0.03%	0.004%
43	8.125	2185	2188	2192	rVB2	287	221	0.03%	0.003%
44	8.173	2192	2203	2222	rBV	82676	140039	16.18%	2.136%
45	8.334	2245	2253	2254	rBV2	392	416	0.05%	0.006%
46	8.363	2260	2262	2266	rVB3	252	146	0.02%	0.002%
47	8.427	2277	2282	2285	rBV2	212	216	0.02%	0.003%
48	8.501	2302	2305	2308	rVB	242	154	0.02%	0.002%
49	8.543	2313	2318	2321	rVB2	230	207	0.02%	0.003%
50	8.578	2325	2329	2331	rBV	248	196	0.02%	0.003%
51	8.630	2333	2345	2379	rVV2	185422	359220	41.51%	5.480%
52	8.916	2431	2434	2437	rBV2	214	147	0.02%	0.002%
53	8.996	2455	2459	2463	rVB2	272	226	0.03%	0.003%
54	9.032	2465	2470	2473	rBV2	194	226	0.03%	0.003%
55	9.054	2473	2477	2480	rVV2	189	167	0.02%	0.003%
56	9.154	2504	2508	2509	rBV	219	150	0.02%	0.002%
57	9.241	2531	2535	2540	rBV2	242	248	0.03%	0.004%
58	9.267	2541	2543	2547	rVV2	203	163	0.02%	0.002%
59	9.411	2576	2588	2610	rBV	351050	593751	68.62%	9.057%
60	9.585	2638	2642	2646	rBV2	260	254	0.03%	0.004%
61	9.701	2676	2678	2682	rVB2	311	170	0.02%	0.003%
62	9.723	2682	2685	2688	rBV	206	172	0.02%	0.003%
63	9.974	2760	2763	2767	rVB	223	185	0.02%	0.003%
64	10.032	2775	2781	2784	rBV2	239	219	0.03%	0.003%
65	10.074	2792	2794	2799	rVB2	232	146	0.02%	0.002%
66	10.141	2812	2815	2821	rVB	286	263	0.03%	0.004%
67	10.340	2874	2877	2879	rBV	223	155	0.02%	0.002%
68	10.411	2896	2899	2903	rVB2	175	156	0.02%	0.002%
69	10.453	2908	2912	2916	rBV2	219	221	0.03%	0.003%
70	10.633	2962	2968	2979	rVB4	1468	2225	0.26%	0.034%
71	10.691	2979	2986	2988	rBV	163	163	0.02%	0.002%
72	10.752	2992	3005	3025	rVB	268720	423946	48.99%	6.467%
73	10.926	3055	3059	3065	rVB2	205	199	0.02%	0.003%
74	10.967	3066	3072	3077	rBV2	250	280	0.03%	0.004%
75	11.070	3099	3104	3107	rBV2	284	297	0.03%	0.005%
76	11.244	3154	3158	3161	rBV2	210	174	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
 Data File : VU053180.D
 Acq On : 02 Mar 2023 12:15
 Operator : JC/MD
 Sample : 01745-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
 Title : VOC Analysis

77	11.344	3186	3189	3192	rBV2	218	174	0.02%	0.003%
78	11.598	3265	3268	3271	rBV	181	158	0.02%	0.002%
79	11.807	3321	3333	3355	rBV	376224	594715	68.73%	9.072%
80	12.000	3385	3393	3397	rBV2	317	509	0.06%	0.008%
81	12.070	3407	3415	3427	rBV5	3255	6368	0.74%	0.097%
82	12.189	3439	3452	3477	rBV	382975	625652	72.30%	9.544%
83	12.527	3553	3557	3564	rVB2	216	226	0.03%	0.003%
84	12.684	3603	3606	3610	rVB2	242	172	0.02%	0.003%
85	12.938	3682	3685	3688	rBV	294	149	0.02%	0.002%
86	12.977	3694	3697	3701	rBV2	277	212	0.02%	0.003%
87	13.463	3844	3848	3850	rBV	236	156	0.02%	0.002%
88	13.623	3895	3898	3904	rVB	376	342	0.04%	0.005%
89	13.652	3904	3907	3909	rBV2	273	178	0.02%	0.003%
90	13.668	3909	3912	3921	rVB	314	297	0.03%	0.005%
91	13.720	3921	3928	3931	rBV2	230	339	0.04%	0.005%
92	13.842	3960	3966	3967	rBV	936	700	0.08%	0.011%
93	14.102	4038	4047	4053	rBV3	548	893	0.10%	0.014%
94	14.186	4071	4073	4075	rBV	256	148	0.02%	0.002%
95	14.331	4112	4118	4119	rBV4	603	552	0.06%	0.008%
96	14.556	4184	4188	4192	rBV2	438	510	0.06%	0.008%
97	14.729	4240	4242	4244	rBV2	324	198	0.02%	0.003%
98	14.742	4244	4246	4252	rVB2	410	319	0.04%	0.005%
99	15.025	4331	4334	4335	rBV	335	151	0.02%	0.002%
100	15.157	4372	4375	4378	rBV2	367	256	0.03%	0.004%




Sum of corrected areas: 6555451

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
Data File : VU053180.D
Acq On : 02 Mar 2023 12:15
Operator : JC/MD
Sample : 01745-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COLF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

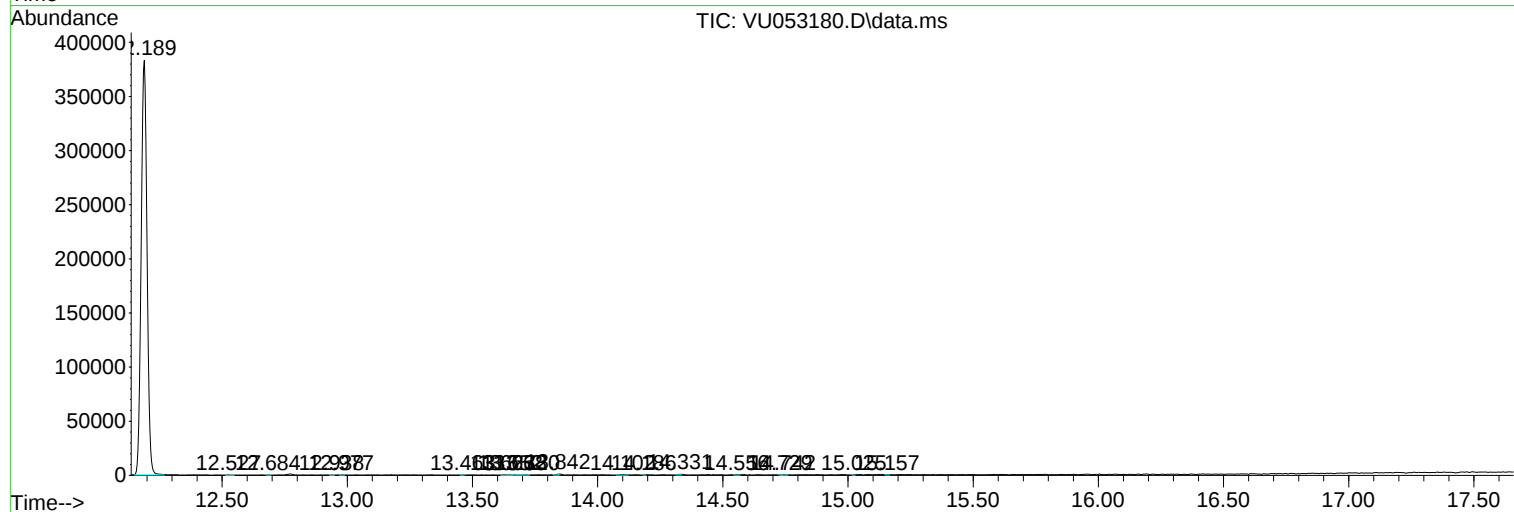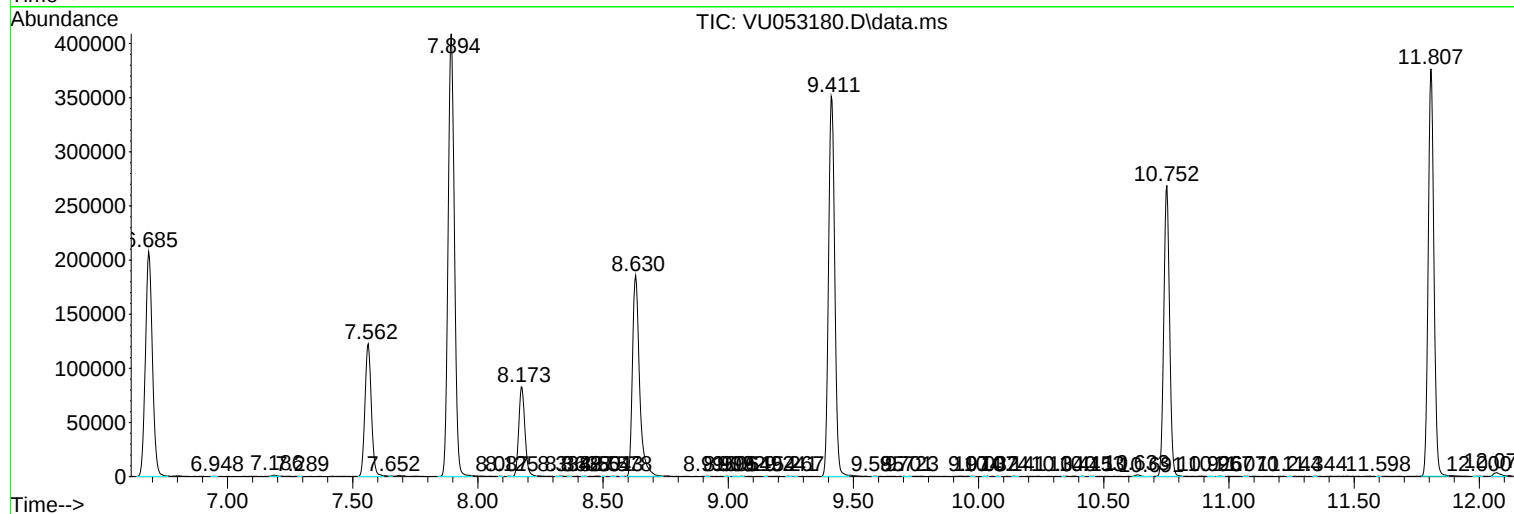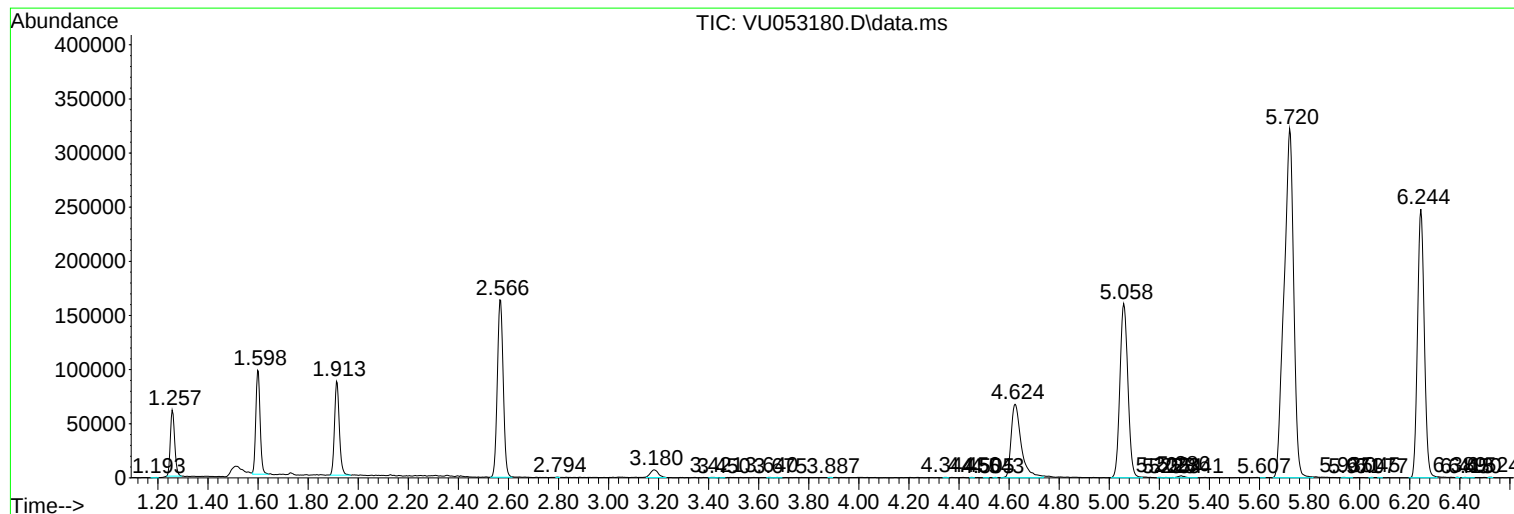

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
Data File : VU053180.D
Acq On : 02 Mar 2023 12:15
Operator : JC/MD
Sample : 01745-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0LF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
Data File : VU053180.D
Acq On : 02 Mar 2023 12:15
Operator : JC/MD
Sample : 01745-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0LF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------