

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
 Data File : VU053185.D
 Acq On : 02 Mar 2023 14:12
 Operator : JC/MD
 Sample : 01745-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLFO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
 Title : VOC Analysis

Signal : TIC: VU053185.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.112	3	7	14	rBV	237	353	0.04%	0.006%
2	1.154	15	20	24	rVV2	191	241	0.03%	0.004%
3	1.193	30	32	33	rVB	106	22	0.00%	0.000%
4	1.257	45	52	70	rVB	60419	72297	9.08%	1.190%
5	1.598	152	158	174	rVB	87341	101285	12.72%	1.667%
6	1.916	249	257	272	rVB	79128	105446	13.24%	1.735%
7	2.566	448	459	476	rVB	149715	243117	30.52%	4.001%
8	3.045	604	608	611	rBV2	503	395	0.05%	0.006%
9	3.183	638	651	666	rBV	6878	15315	1.92%	0.252%
10	4.148	948	951	955	rBV	226	149	0.02%	0.002%
11	4.241	976	980	986	rVB2	239	245	0.03%	0.004%
12	4.444	1040	1043	1048	rVB	288	184	0.02%	0.003%
13	4.627	1084	1100	1134	rBV2	64704	181259	22.76%	2.983%
14	4.910	1186	1188	1189	rBV	215	72	0.01%	0.001%
15	4.958	1201	1203	1206	rVB	202	104	0.01%	0.002%
16	5.058	1218	1234	1258	rBV	149983	328778	41.27%	5.410%
17	5.286	1297	1305	1320	rVB5	1621	3423	0.43%	0.056%
18	5.556	1388	1389	1390	rBV5	108	22	0.00%	0.000%
19	5.720	1419	1440	1463	rBV2	291970	796564	100.00%	13.108%
20	5.939	1507	1508	1510	rVB	170	62	0.01%	0.001%
21	5.964	1513	1516	1519	rBV2	334	267	0.03%	0.004%
22	6.087	1551	1554	1556	rBV	209	112	0.01%	0.002%
23	6.244	1590	1603	1621	rBV	229557	437726	54.95%	7.203%
24	6.431	1658	1661	1663	rVB2	187	107	0.01%	0.002%
25	6.450	1663	1667	1670	rBV	210	234	0.03%	0.004%
26	6.501	1681	1683	1686	rBV	328	174	0.02%	0.003%
27	6.524	1687	1690	1695	rVV4	630	477	0.06%	0.008%
28	6.607	1714	1716	1718	rBV	227	106	0.01%	0.002%
29	6.685	1727	1740	1765	rVB	189350	366591	46.02%	6.032%
30	6.800	1773	1776	1777	rBV	266	153	0.02%	0.003%
31	7.144	1880	1883	1885	rBV	236	162	0.02%	0.003%
32	7.189	1889	1897	1906	rVV5	1321	2167	0.27%	0.036%
33	7.440	1972	1975	1979	rBV	254	247	0.03%	0.004%
34	7.559	2000	2012	2036	rBV	108955	195561	24.55%	3.218%
35	7.665	2042	2045	2047	rBV2	262	192	0.02%	0.003%
36	7.781	2079	2081	2087	rVB	249	138	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
 Data File : VU053185.D
 Acq On : 02 Mar 2023 14:12
 Operator : JC/MD
 Sample : 01745-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLFO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
 Title : VOC Analysis

37	7.813	2088	2091	2093	rVB2	184	108	0.01%	0.002%
38	7.894	2102	2116	2138	rBV	377559	649673	81.56%	10.691%
39	8.064	2166	2169	2172	rBV2	297	258	0.03%	0.004%
40	8.096	2177	2179	2180	rBV2	100	26	0.00%	0.000%
41	8.173	2192	2203	2224	rBV2	76599	128940	16.19%	2.122%
42	8.279	2234	2236	2238	rVB	191	62	0.01%	0.001%
43	8.385	2267	2269	2271	rBV	180	112	0.01%	0.002%
44	8.443	2283	2287	2289	rBV2	201	175	0.02%	0.003%
45	8.501	2304	2305	2307	rBV2	104	42	0.01%	0.001%
46	8.630	2334	2345	2376	rBV2	180938	343794	43.16%	5.657%
47	8.948	2441	2444	2448	rBV2	235	179	0.02%	0.003%
48	8.971	2448	2451	2453	rBV2	203	118	0.01%	0.002%
49	9.135	2500	2502	2504	rBV	146	67	0.01%	0.001%
50	9.164	2508	2511	2513	rBV	208	112	0.01%	0.002%
51	9.238	2532	2534	2536	rBV2	215	141	0.02%	0.002%
52	9.353	2567	2570	2572	rBV	254	189	0.02%	0.003%
53	9.411	2576	2588	2616	rBV	327035	548926	68.91%	9.033%
54	9.559	2632	2634	2636	rVB	216	107	0.01%	0.002%
55	9.630	2654	2656	2657	rBV	157	68	0.01%	0.001%
56	9.717	2682	2683	2684	rBV	126	33	0.00%	0.001%
57	9.942	2751	2753	2756	rVB2	193	102	0.01%	0.002%
58	9.996	2767	2770	2773	rBV2	217	153	0.02%	0.003%
59	10.633	2963	2968	2980	rVB4	1112	1741	0.22%	0.029%
60	10.752	2993	3005	3024	rVB	251701	401177	50.36%	6.602%
61	11.173	3134	3136	3138	rBV	171	98	0.01%	0.002%
62	11.681	3291	3294	3301	rVB	208	150	0.02%	0.002%
63	11.729	3308	3309	3314	rVB	171	108	0.01%	0.002%
64	11.807	3321	3333	3350	rBV	360860	566085	71.07%	9.315%
65	11.922	3366	3369	3373	rVB	408	216	0.03%	0.004%
66	12.067	3411	3414	3416	rBV	1023	784	0.10%	0.013%
67	12.189	3439	3452	3468	rBV	356748	578030	72.57%	9.512%
68	12.366	3504	3507	3509	rBV	256	151	0.02%	0.002%
69	13.498	3856	3859	3862	rBV	263	193	0.02%	0.003%
70	13.942	3995	3997	4000	rVB2	346	157	0.02%	0.003%
71	14.102	4044	4047	4049	rBV	266	188	0.02%	0.003%
72	14.430	4147	4149	4152	rBV	314	201	0.03%	0.003%
73	14.491	4165	4168	4172	rBV	305	248	0.03%	0.004%
74	14.540	4181	4183	4186	rVB2	455	235	0.03%	0.004%
75	14.954	4310	4312	4313	rBV2	250	109	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
Data File : VU053185.D
Acq On : 02 Mar 2023 14:12
Operator : JC/MD
Sample : 01745-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COLFO

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Title : VOC Analysis


Sum of corrected areas: 6077003

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
Data File : VU053185.D
Acq On : 02 Mar 2023 14:12
Operator : JC/MD
Sample : 01745-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COLFO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

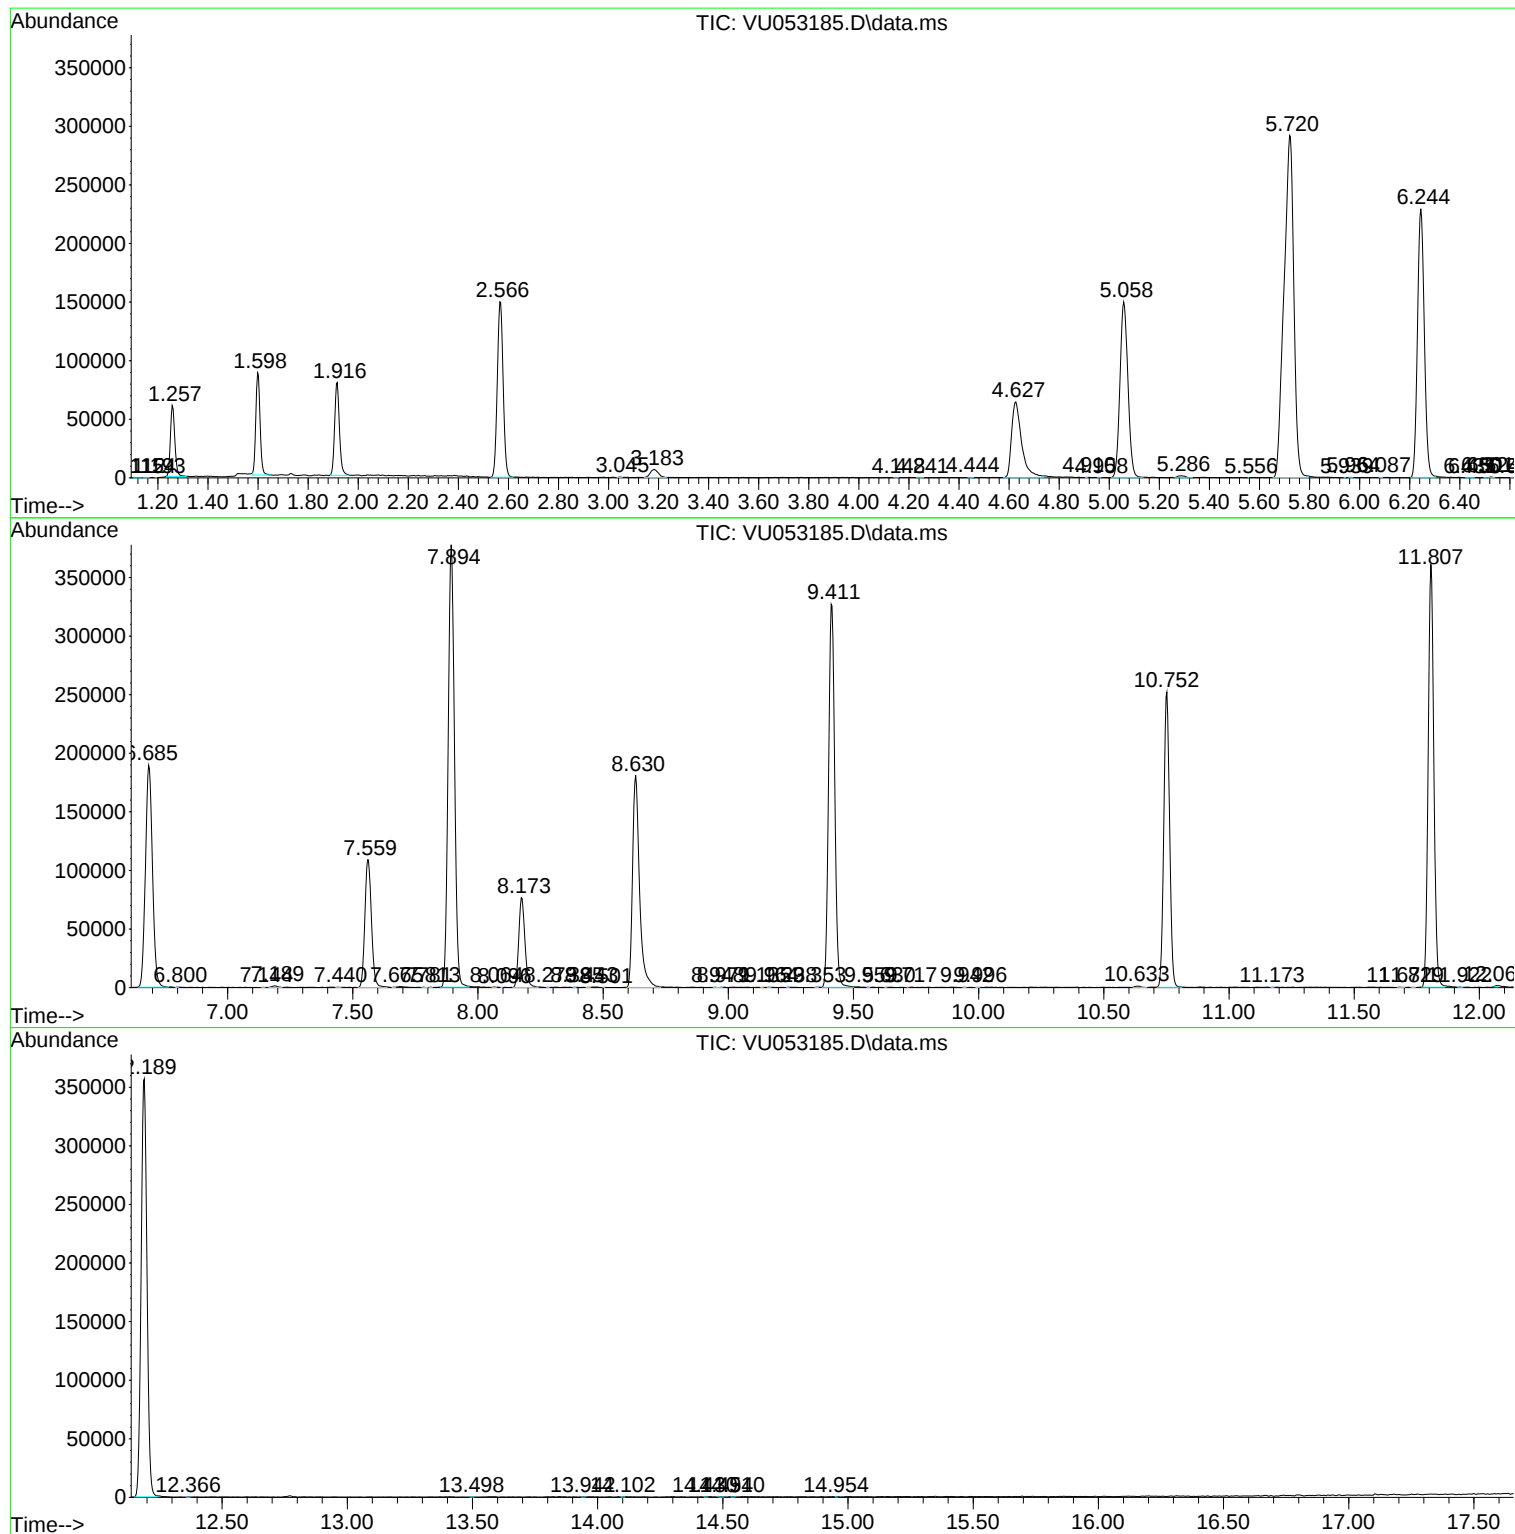

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
Data File : VU053185.D
Acq On : 02 Mar 2023 14:12
Operator : JC/MD
Sample : 01745-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COLFO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
Data File : VU053185.D
Acq On : 02 Mar 2023 14:12
Operator : JC/MD
Sample : 01745-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COLFO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------