

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
 Data File : VU053186.D
 Acq On : 02 Mar 2023 14:35
 Operator : JC/MD
 Sample : 01745-05 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLF2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
 Title : VOC Analysis

Signal : TIC: VU053186.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.122	3	10	14	rBV	306	369	0.02%	0.004%
2	1.154	17	20	21	rVV	146	83	0.00%	0.001%
3	1.180	25	28	31	rBV2	192	138	0.01%	0.001%
4	1.257	44	52	72	rVB	161925	198628	8.23%	1.902%
5	1.598	151	158	178	rVB	87814	102422	4.24%	0.981%
6	1.913	248	256	278	rVB	81504	110069	4.56%	1.054%
7	2.566	448	459	476	rVB	152866	246614	10.22%	2.361%
8	3.701	809	812	813	rBV	218	99	0.00%	0.001%
9	4.100	933	936	939	rVB2	255	153	0.01%	0.001%
10	4.219	970	973	975	rVB	215	115	0.00%	0.001%
11	4.408	1029	1032	1035	rBV2	222	147	0.01%	0.001%
12	4.428	1035	1038	1040	rBV	176	132	0.01%	0.001%
13	4.463	1045	1049	1051	rBV	311	271	0.01%	0.003%
14	4.553	1075	1077	1083	rBV	180	138	0.01%	0.001%
15	4.624	1086	1099	1130	rBV	56822	151553	6.28%	1.451%
16	4.878	1176	1178	1184	rBV	176	136	0.01%	0.001%
17	4.974	1206	1208	1209	rBV	143	40	0.00%	0.000%
18	5.058	1219	1234	1260	rBV	152211	330101	13.68%	3.160%
19	5.286	1295	1305	1306	rBV4	1281	1707	0.07%	0.016%
20	5.331	1316	1319	1327	rBV	106	134	0.01%	0.001%
21	5.379	1327	1334	1335	rBV	586	432	0.02%	0.004%
22	5.476	1362	1364	1367	rBV	207	129	0.01%	0.001%
23	5.521	1372	1378	1389	rBV3	674	1158	0.05%	0.011%
24	5.720	1418	1440	1450	rBV2	296444	831076	34.43%	7.956%
25	5.910	1495	1499	1504	rBV	318	265	0.01%	0.003%
26	6.106	1558	1560	1563	rBV2	276	147	0.01%	0.001%
27	6.244	1590	1603	1624	rBV	232118	437526	18.13%	4.189%
28	6.402	1648	1652	1655	rBV3	226	232	0.01%	0.002%
29	6.495	1678	1681	1683	rVB2	290	136	0.01%	0.001%
30	6.521	1686	1689	1690	rBV2	395	242	0.01%	0.002%
31	6.685	1727	1740	1760	rBV	191611	371508	15.39%	3.557%
32	6.807	1771	1778	1782	rBV2	561	602	0.02%	0.006%
33	7.183	1889	1895	1907	rVB3	1219	1993	0.08%	0.019%
34	7.302	1930	1932	1935	rBV2	182	98	0.00%	0.001%
35	7.360	1948	1950	1952	rBV	135	60	0.00%	0.001%
36	7.373	1952	1954	1958	rBV	195	107	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
 Data File : VU053186.D
 Acq On : 02 Mar 2023 14:35
 Operator : JC/MD
 Sample : 01745-05 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLF2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
 Title : VOC Analysis

37	7.399	1960	1962	1965	rBV2	201	141	0.01%	0.001%
38	7.514	1996	1998	2000	rBV	230	162	0.01%	0.002%
39	7.559	2000	2012	2031	rVV2	110154	197025	8.16%	1.886%
40	7.691	2046	2053	2061	rBV4	824	1322	0.05%	0.013%
41	7.894	2102	2116	2146	rBV	388392	668457	27.69%	6.399%
42	8.083	2171	2175	2180	rBV2	272	250	0.01%	0.002%
43	8.106	2180	2182	2186	rVB	217	140	0.01%	0.001%
44	8.173	2192	2203	2221	rBV	76185	130879	5.42%	1.253%
45	8.308	2242	2245	2248	rVB3	268	201	0.01%	0.002%
46	8.395	2270	2272	2275	rBV	156	79	0.00%	0.001%
47	8.434	2282	2284	2286	rBV	171	104	0.00%	0.001%
48	8.463	2291	2293	2295	rBV2	317	164	0.01%	0.002%
49	8.495	2300	2303	2306	rBV	249	140	0.01%	0.001%
50	8.514	2307	2309	2311	rBV	171	73	0.00%	0.001%
51	8.630	2333	2345	2378	rBV2	182144	348456	14.44%	3.336%
52	8.862	2414	2417	2418	rBV2	182	97	0.00%	0.001%
53	9.090	2486	2488	2489	rBV2	149	42	0.00%	0.000%
54	9.440	2575	2597	2626	rBV2	1138239	2413763	100.00%	23.108%
55	9.910	2741	2743	2744	rBV	157	63	0.00%	0.001%
56	10.025	2777	2779	2781	rBV	199	89	0.00%	0.001%
57	10.392	2888	2893	2896	rVB2	273	253	0.01%	0.002%
58	10.443	2907	2909	2910	rBV2	136	39	0.00%	0.000%
59	10.636	2961	2969	2978	rVB4	1442	1995	0.08%	0.019%
60	10.752	2992	3005	3022	rBV	252521	405092	16.78%	3.878%
61	10.849	3032	3035	3038	rBV2	247	189	0.01%	0.002%
62	11.112	3114	3117	3120	rBV	322	182	0.01%	0.002%
63	11.241	3155	3157	3160	rBV	224	135	0.01%	0.001%
64	11.289	3167	3172	3175	rBV	236	180	0.01%	0.002%
65	11.742	3302	3313	3322	rBV	68109	106493	4.41%	1.020%
66	11.829	3322	3340	3363	rVB2	578974	1456799	60.35%	13.947%
67	11.951	3376	3378	3382	rBV	288	214	0.01%	0.002%
68	12.205	3439	3457	3487	rBV2	768974	1702863	70.55%	16.302%
69	13.263	3783	3786	3791	rBV	250	161	0.01%	0.002%
70	13.357	3812	3815	3818	rBV	223	145	0.01%	0.001%
71	13.836	3953	3964	3986	rVB	115580	183855	7.62%	1.760%
72	13.993	4011	4013	4018	rVB	308	157	0.01%	0.002%
73	14.122	4050	4053	4058	rBB	364	226	0.01%	0.002%
74	14.328	4108	4117	4128	rBV2	22650	35538	1.47%	0.340%
75	14.845	4275	4278	4280	rBV	319	224	0.01%	0.002%
76	14.900	4293	4295	4298	rBV	247	110	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
Data File : VU053186.D
Acq On : 02 Mar 2023 14:35
Operator : JC/MD
Sample : 01745-05 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0LF2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Title : VOC Analysis

77	14.987	4319	4322	4326	rBV2	364	268	0.01%	0.003%
----	--------	------	------	------	------	-----	-----	-------	--------




Sum of corrected areas: 10445525

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
Data File : VU053186.D
Acq On : 02 Mar 2023 14:35
Operator : JC/MD
Sample : 01745-05 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COLF2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

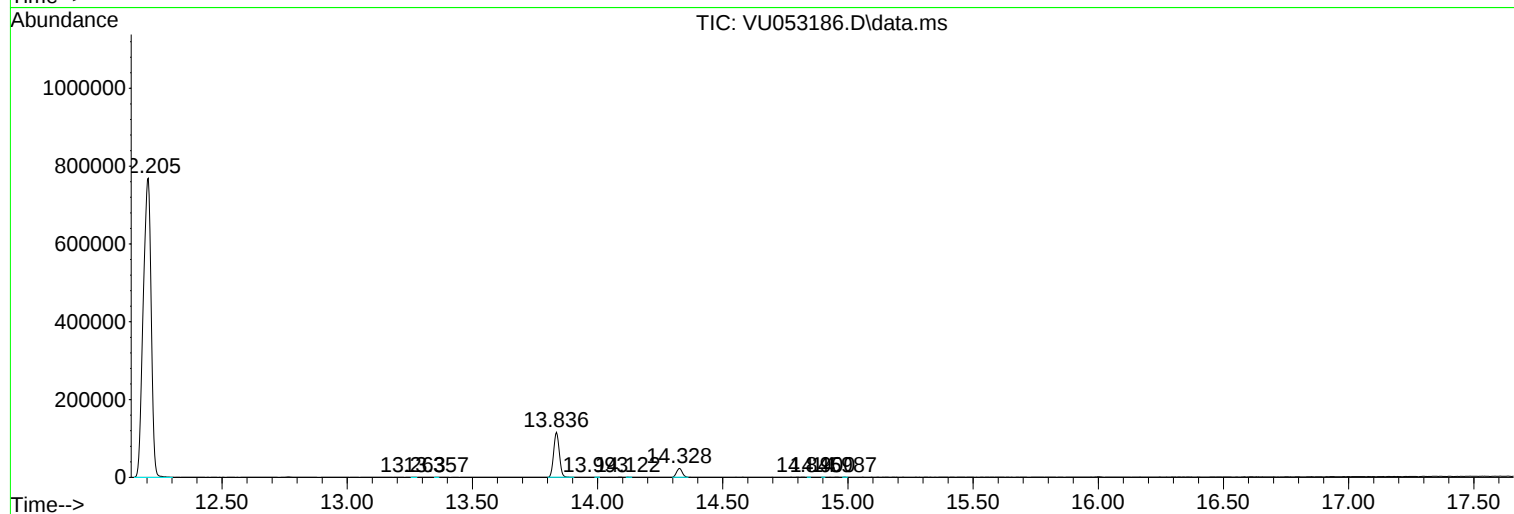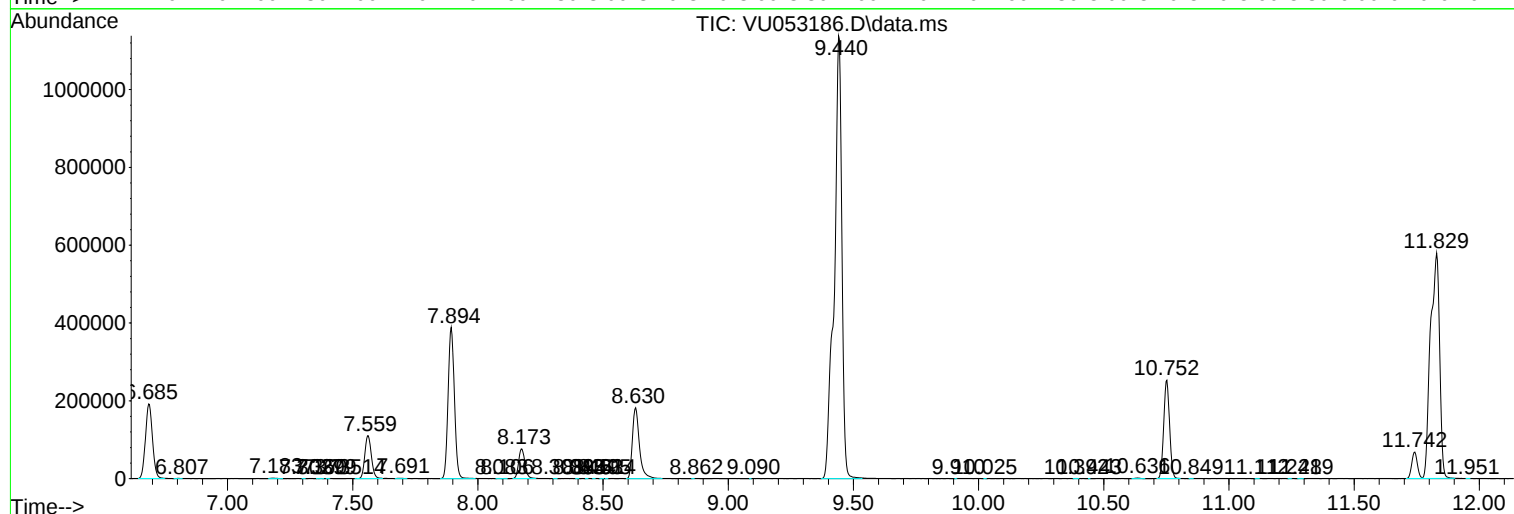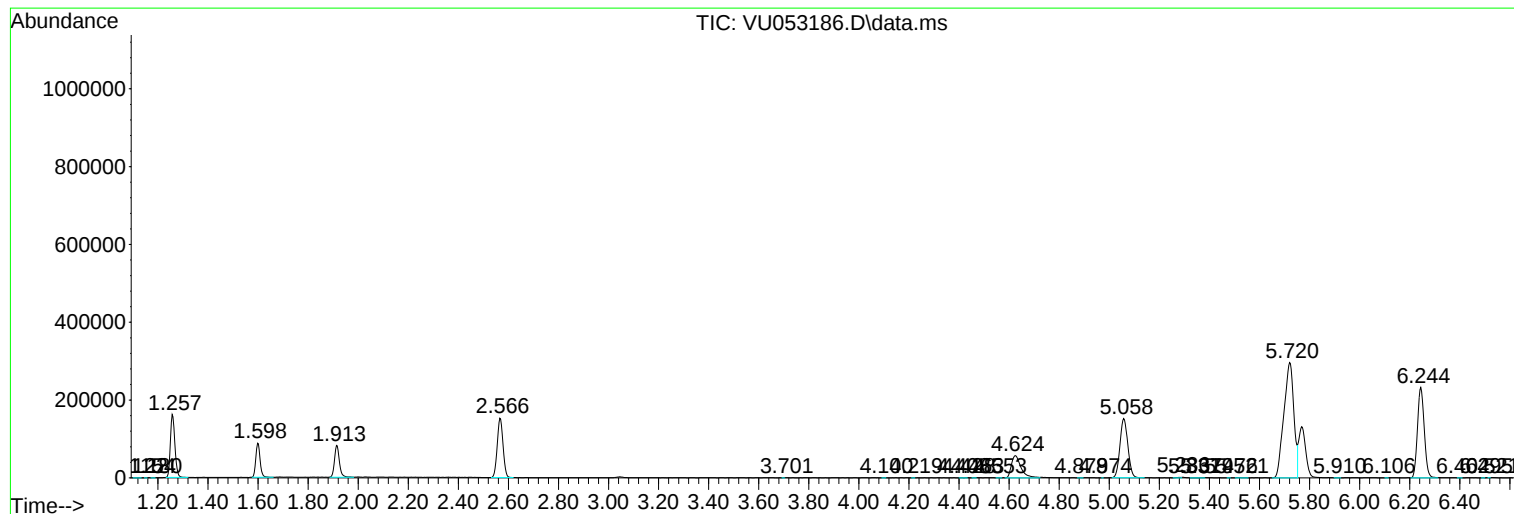

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
Data File : VU053186.D
Acq On : 02 Mar 2023 14:35
Operator : JC/MD
Sample : 01745-05 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0LF2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
Data File : VU053186.D
Acq On : 02 Mar 2023 14:35
Operator : JC/MD
Sample : 01745-05 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0LF2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------