

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
 Data File : VU053187.D
 Acq On : 02 Mar 2023 15:13
 Operator : JC/MD
 Sample : 01745-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
 Title : VOC Analysis

Signal : TIC: VU053187.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.113	6	7	8	rBV	117	28	0.00%	0.000%
2	1.145	14	17	21	rVB	232	180	0.02%	0.003%
3	1.164	21	23	25	rBV	124	54	0.01%	0.001%
4	1.257	44	52	70	rBV	153958	198765	23.82%	3.144%
5	1.598	151	158	171	rBV	92259	105254	12.62%	1.665%
6	1.913	249	256	275	rVB	83523	110944	13.30%	1.755%
7	2.566	447	459	475	rBV	159415	258522	30.99%	4.089%
8	3.010	596	597	601	rBV	168	120	0.01%	0.002%
9	3.048	601	609	615	rVB4	1060	1671	0.20%	0.026%
10	3.129	632	634	637	rVB2	254	140	0.02%	0.002%
11	3.338	696	699	700	rBV2	171	82	0.01%	0.001%
12	4.006	904	907	909	rBV	178	81	0.01%	0.001%
13	4.103	935	937	940	rVB2	248	133	0.02%	0.002%
14	4.209	967	970	973	rBV2	213	141	0.02%	0.002%
15	4.302	997	999	1002	rBV	208	132	0.02%	0.002%
16	4.540	1068	1073	1078	rBV2	243	230	0.03%	0.004%
17	4.627	1087	1100	1128	rBV	57317	153654	18.42%	2.430%
18	4.910	1185	1188	1189	rBV	179	107	0.01%	0.002%
19	5.058	1219	1234	1260	rVB	153665	335006	40.15%	5.299%
20	5.411	1342	1344	1345	rBV	131	56	0.01%	0.001%
21	5.469	1359	1362	1366	rVB	259	187	0.02%	0.003%
22	5.495	1366	1370	1373	rBV	216	171	0.02%	0.003%
23	5.527	1379	1380	1381	rBV	110	29	0.00%	0.000%
24	5.598	1400	1402	1404	rBV	175	96	0.01%	0.002%
25	5.617	1406	1408	1412	rVB	182	84	0.01%	0.001%
26	5.720	1420	1440	1465	rBV2	304893	834295	100.00%	13.196%
27	5.993	1524	1525	1529	rVB2	243	74	0.01%	0.001%
28	6.042	1536	1540	1541	rBV3	391	265	0.03%	0.004%
29	6.244	1590	1603	1623	rBV	226339	427444	51.23%	6.761%
30	6.408	1653	1654	1661	rBV	132	88	0.01%	0.001%
31	6.466	1668	1672	1680	rVB2	348	534	0.06%	0.008%
32	6.688	1727	1741	1766	rBV	196543	382751	45.88%	6.054%
33	6.897	1805	1806	1808	rVB	169	62	0.01%	0.001%
34	7.035	1843	1849	1851	rBV	217	224	0.03%	0.004%
35	7.074	1859	1861	1863	rVB	171	68	0.01%	0.001%
36	7.087	1863	1865	1868	rVB	164	73	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
 Data File : VU053187.D
 Acq On : 02 Mar 2023 15:13
 Operator : JC/MD
 Sample : 01745-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
 Title : VOC Analysis

37	7.103	1868	1870	1873	rBV	134	53	0.01%	0.001%
38	7.122	1873	1876	1877	rBV	145	61	0.01%	0.001%
39	7.145	1881	1883	1888	rBV2	234	184	0.02%	0.003%
40	7.186	1888	1896	1903	rBV3	1304	2001	0.24%	0.032%
41	7.254	1916	1917	1920	rBV	105	40	0.00%	0.001%
42	7.453	1977	1979	1983	rBV	124	45	0.01%	0.001%
43	7.562	2001	2013	2033	rBV2	115985	202044	24.22%	3.196%
44	7.681	2046	2050	2052	rBV	643	463	0.06%	0.007%
45	7.894	2102	2116	2136	rBV	395904	683064	81.87%	10.804%
46	8.177	2192	2204	2226	rBV	77279	133231	15.97%	2.107%
47	8.308	2243	2245	2248	rBV	135	47	0.01%	0.001%
48	8.543	2316	2318	2320	rBV	155	45	0.01%	0.001%
49	8.585	2328	2331	2334	rBV	180	87	0.01%	0.001%
50	8.630	2334	2345	2380	rBV3	181846	350457	42.01%	5.543%
51	8.871	2417	2420	2423	rBV	221	101	0.01%	0.002%
52	9.074	2481	2483	2485	rBV	130	64	0.01%	0.001%
53	9.251	2535	2538	2541	rBV	186	112	0.01%	0.002%
54	9.415	2576	2589	2614	rBV	325857	541128	64.86%	8.559%
55	9.591	2642	2644	2649	rVB	205	109	0.01%	0.002%
56	9.768	2696	2699	2701	rBV	148	110	0.01%	0.002%
57	9.842	2719	2722	2727	rBV2	170	163	0.02%	0.003%
58	9.878	2730	2733	2739	rBV2	209	202	0.02%	0.003%
59	9.964	2758	2760	2763	rBV	201	99	0.01%	0.002%
60	10.077	2792	2795	2797	rBV	171	84	0.01%	0.001%
61	10.144	2814	2816	2822	rVB	143	77	0.01%	0.001%
62	10.173	2822	2825	2826	rBV	169	78	0.01%	0.001%
63	10.344	2876	2878	2880	rBB	146	59	0.01%	0.001%
64	10.424	2898	2903	2906	rBV2	214	199	0.02%	0.003%
65	10.636	2965	2969	2975	rVB4	950	1151	0.14%	0.018%
66	10.752	2993	3005	3025	rBV	257563	406394	48.71%	6.428%
67	11.286	3169	3171	3173	rBV	158	47	0.01%	0.001%
68	11.305	3174	3177	3180	rBV2	225	132	0.02%	0.002%
69	11.376	3195	3199	3204	rVB	290	231	0.03%	0.004%
70	11.636	3276	3280	3282	rBV2	299	185	0.02%	0.003%
71	11.810	3322	3334	3359	rBV	345981	563528	67.55%	8.913%
72	12.189	3439	3452	3475	rBV	375952	615270	73.75%	9.732%
73	12.630	3587	3589	3590	rBV	123	29	0.00%	0.000%
74	12.755	3624	3628	3629	rBV	438	305	0.04%	0.005%
75	13.845	3958	3967	3979	rBV4	4465	7224	0.87%	0.114%
76	14.327	4114	4117	4125	rVB4	935	962	0.12%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
Data File : VU053187.D
Acq On : 02 Mar 2023 15:13
Operator : JC/MD
Sample : 01745-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Title : VOC Analysis

77	14.903	4294	4296	4300	rBV2	403	290	0.03%	0.005%
78	15.202	4386	4389	4392	rBV	486	330	0.04%	0.005%


Sum of corrected areas: 6322230

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
Data File : VU053187.D
Acq On : 02 Mar 2023 15:13
Operator : JC/MD
Sample : 01745-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

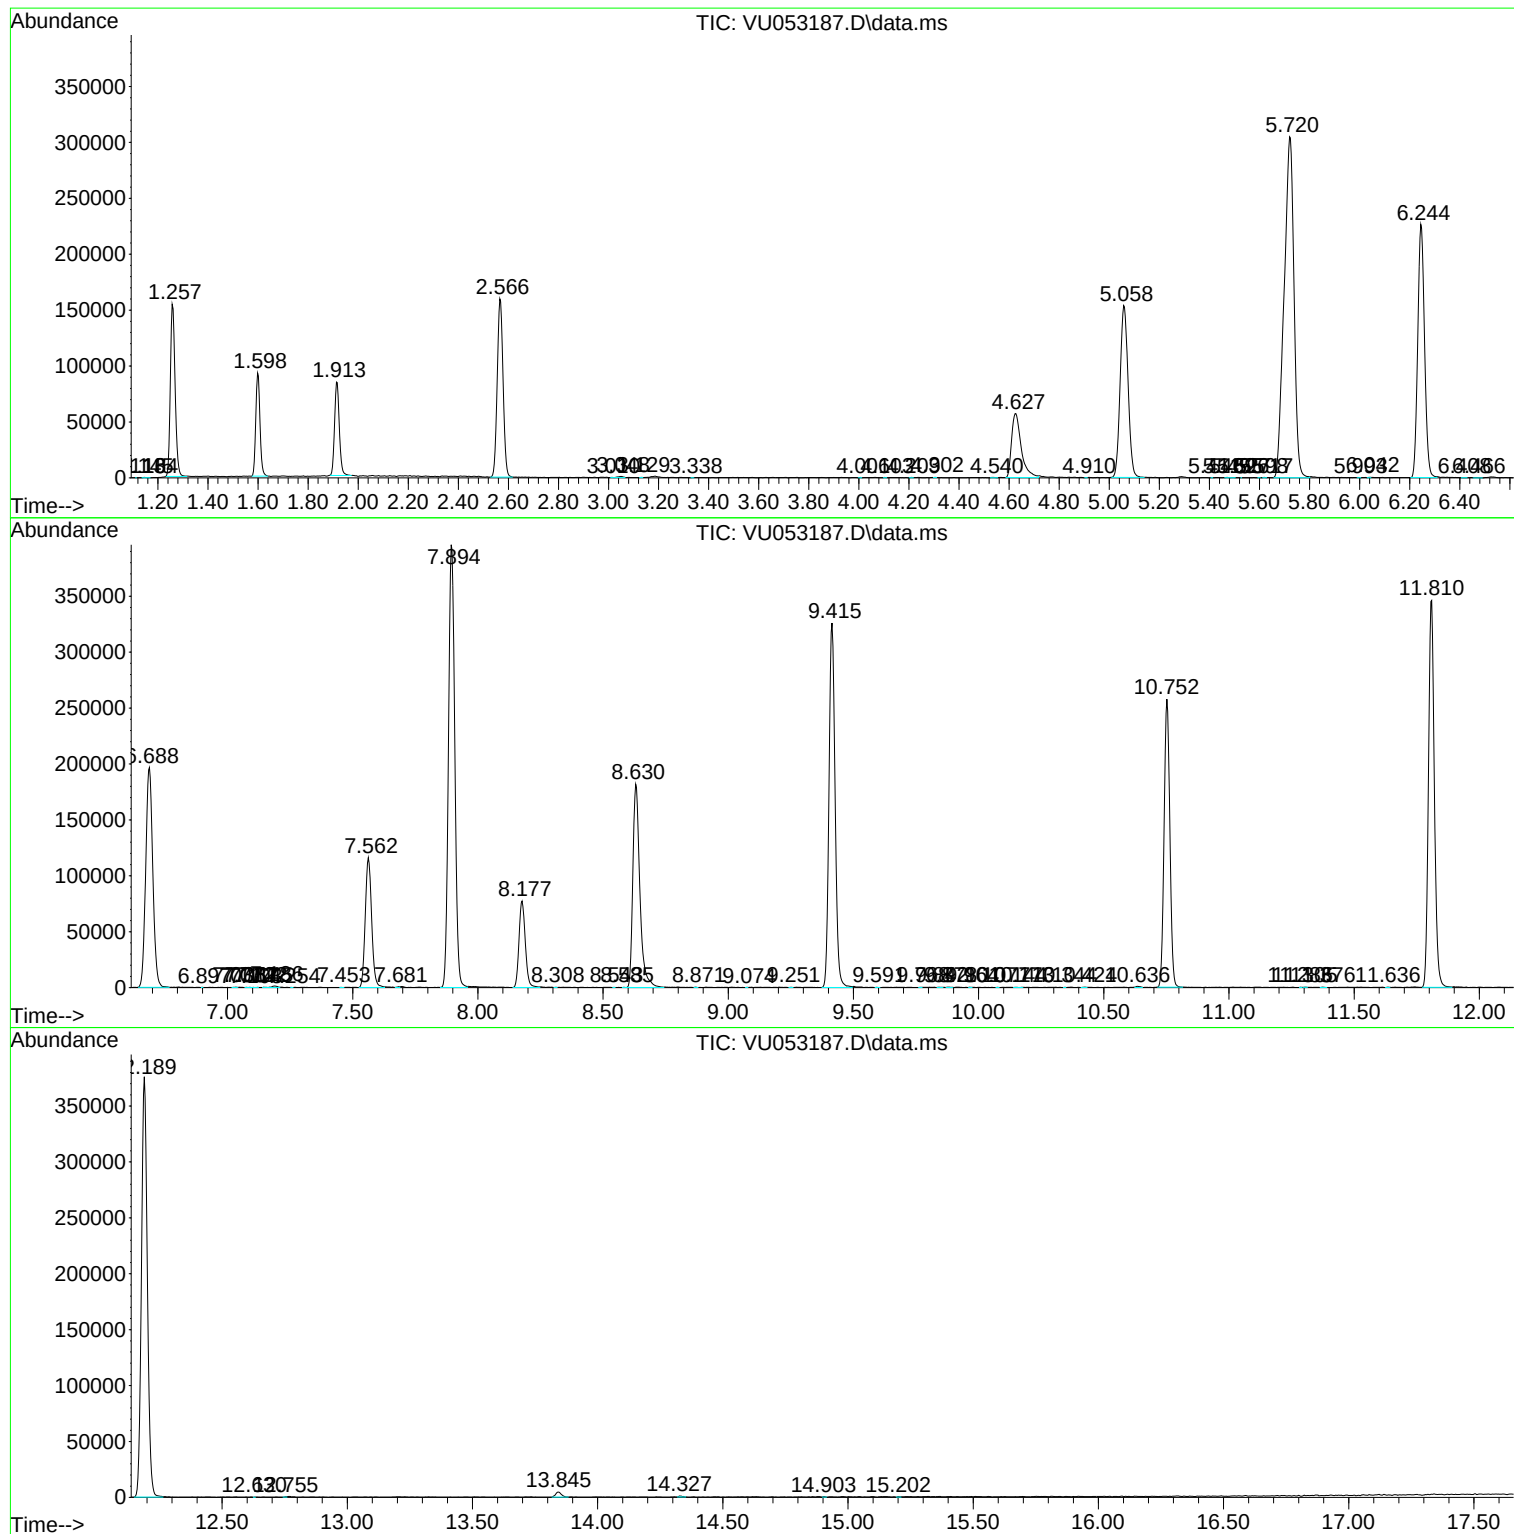

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
Data File : VU053187.D
Acq On : 02 Mar 2023 15:13
Operator : JC/MD
Sample : 01745-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
Data File : VU053187.D
Acq On : 02 Mar 2023 15:13
Operator : JC/MD
Sample : 01745-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------