


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030223\
Data File : VU053174.D
Acq On : 02 Mar 2023 09:11
Operator : JC/MD
Sample : BFB162
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB162

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Title : VOC Analysis
Last Update : Fri Mar 03 01:44:16 2023

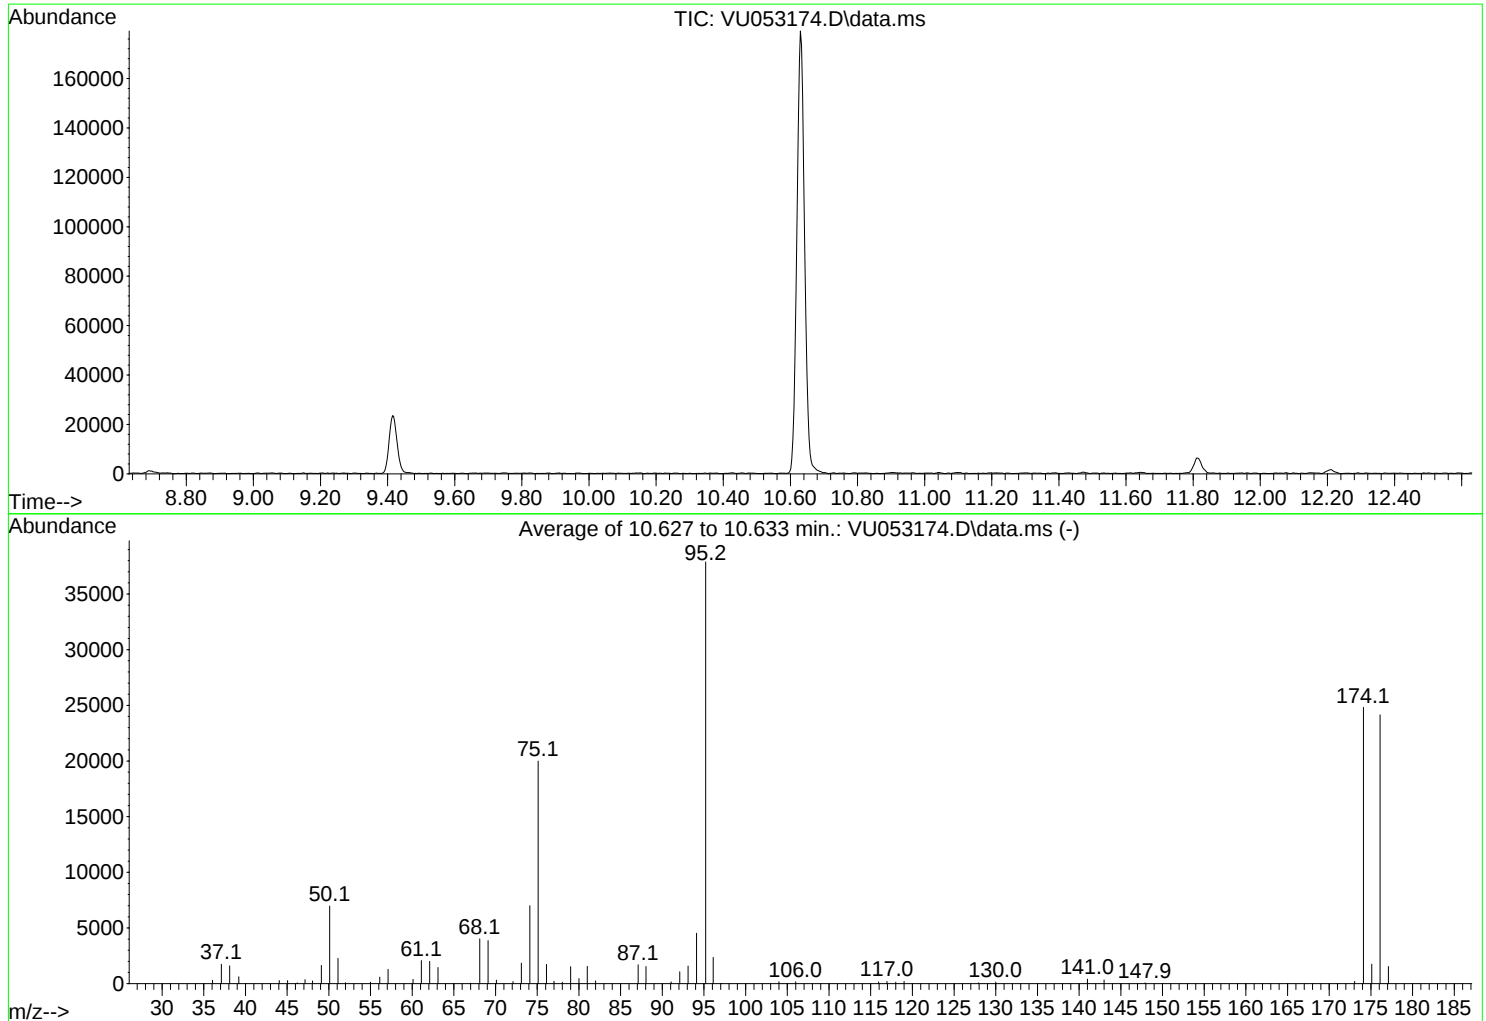

AutoFind: Scans 2966, 2967, 2968; Background Corrected with Scan 2955

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	6973	PASS
75	95	30	80	52.8	19995	PASS
95	95	100	100	100.0	37891	PASS
96	95	5	9	6.2	2361	PASS
173	174	0.00	2	0.8	204	PASS
174	95	50	120	65.5	24819	PASS
175	174	5	9	7.1	1756	PASS
176	174	95	101	97.3	24155	PASS
177	176	5	9	6.4	1543	PASS

m/z	Abundance
40.00	108.0
44.10	207.0

Instrument :
MSVOA_U
ClientSampleId :
BFB162

m/z	Abundance
36.00	321.0
37.10	1735.0
38.10	1579.0
39.20	667.0
40.10	102.0
44.00	452.0
45.00	276.0
46.20	109.0
47.10	341.0
48.10	234.0
49.10	1574.0
50.10	6810.0
51.10	2125.0
55.00	124.0
56.10	637.0
57.10	1208.0
60.10	343.0
61.10	1985.0
62.10	1956.0
63.10	1386.0
67.00	134.0
68.10	3792.0
69.10	3847.0
70.10	311.0
72.10	177.0
73.10	1777.0
74.10	6918.0
75.10	19600.0
76.10	1793.0
77.00	146.0
78.00	122.0
79.00	1355.0
80.00	409.0
81.00	1497.0
82.00	197.0
87.10	1671.0
88.10	1497.0
91.10	189.0
92.10	996.0
93.10	1559.0
94.10	4424.0
95.20	36568.0
96.10	2240.0
104.00	167.0
106.00	136.0
115.90	153.0
117.00	207.0
118.00	146.0
119.00	216.0
127.90	118.0
130.00	118.0
141.00	393.0
143.00	316.0
147.90	105.0
173.10	192.0
174.10	23392.0
175.10	1695.0
176.10	22944.0
177.10	1536.0

Instrument :
MSVOA_U
ClientSampleId :
BFB162

m/z	Abundance
36.10	315.0
37.10	1815.0
38.10	1678.0
39.20	656.0
40.10	123.0
44.10	488.0
45.10	283.0
46.20	115.0
47.20	370.0
48.10	250.0
49.10	1696.0
50.10	7169.0
51.10	2351.0
52.00	120.0
55.00	152.0
56.10	601.0
57.10	1334.0
60.10	410.0
61.10	2156.0
62.10	2101.0
63.10	1481.0
68.10	4133.0
69.10	3989.0
70.10	322.0
72.10	191.0
73.10	1898.0
74.10	7242.0
75.10	20640.0
76.10	1809.0
77.00	211.0
78.00	124.0
79.00	1594.0
80.00	476.0
81.00	1627.0
82.00	233.0
87.10	1765.0
88.10	1609.0
91.10	151.0
92.10	1091.0
93.10	1612.0
94.10	4659.0
95.20	39184.0
96.10	2438.0
97.10	100.0
104.00	171.0
106.00	179.0
115.90	143.0
117.00	200.0
118.00	144.0
119.00	215.0
127.90	108.0
130.00	153.0
141.00	418.0
143.00	336.0
147.90	104.0
173.00	202.0
174.10	25680.0
175.10	1806.0
176.10	24960.0
177.10	1596.0

Instrument :
MSVOA_U
ClientSampleId :
BFB162

m/z	Abundance
36.10	279.0
37.10	1672.0
38.10	1541.0
39.20	551.0
40.10	123.0
44.10	510.0
45.10	280.0
47.20	359.0
48.00	233.0
49.10	1626.0
50.10	6939.0
51.10	2349.0
52.00	145.0
55.00	133.0
56.10	537.0
57.10	1286.0
60.10	414.0
61.10	2057.0
62.10	1943.0
63.10	1509.0
68.10	4169.0
69.10	3788.0
70.10	297.0
72.10	191.0
73.10	1864.0
74.10	6847.0
75.10	19744.0
76.10	1570.0
77.00	292.0
78.00	139.0
79.00	1626.0
80.00	477.0
81.00	1547.0
82.00	290.0
87.10	1633.0
88.00	1517.0
90.90	138.0
92.10	1123.0
93.10	1593.0
94.10	4500.0
95.20	37920.0
96.10	2406.0
104.00	164.0
106.00	195.0
116.00	131.0
116.90	213.0
118.00	120.0
119.00	177.0
130.00	158.0
141.00	380.0
143.00	358.0
173.00	218.0
174.10	25384.0
175.10	1768.0
176.10	24560.0
177.10	1497.0

Instrument :
MSVOA_U
ClientSampleId :
BFB162