

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU030320\
 Data File : VU037019.D
 Acq On : 03 Mar 2020 13:27
 Operator : JC/MD
 Sample : VU0303WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK37

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	78	85	100	rVB	163723	175076	15.37%	2.131%
2	1.925	175	182	194	rVB	136577	180173	15.82%	2.193%
3	2.591	376	389	406	rBV	228185	376657	33.08%	4.584%
4	2.819	459	460	462	rBV	219	104	0.01%	0.001%
5	2.922	490	492	494	rVB	192	62	0.01%	0.001%
6	2.964	503	505	512	rBV2	268	239	0.02%	0.003%
7	3.112	547	551	552	rBV	212	129	0.01%	0.002%
8	3.179	570	572	574	rBV	121	51	0.00%	0.001%
9	3.208	579	581	583	rBV	135	49	0.00%	0.001%
10	3.269	597	600	603	rBV2	181	128	0.01%	0.002%
11	3.337	618	621	624	rBV2	186	126	0.01%	0.002%
12	3.459	656	659	661	rBV	243	165	0.01%	0.002%
13	3.488	665	668	671	rVV	240	168	0.01%	0.002%
14	3.504	671	673	676	rVB	167	71	0.01%	0.001%
15	3.693	727	732	736	rVB	252	302	0.03%	0.004%
16	3.726	740	742	743	rBV	97	39	0.00%	0.000%
17	3.758	748	752	754	rBV	228	170	0.01%	0.002%
18	3.809	764	768	773	rVB	88	80	0.01%	0.001%
19	3.851	778	781	784	rBV2	259	124	0.01%	0.002%
20	3.928	803	805	808	rBV	77	50	0.00%	0.001%
21	3.941	808	809	810	rBV	97	35	0.00%	0.000%
22	4.140	868	871	873	rBV2	202	121	0.01%	0.001%
23	4.153	873	875	876	rVV2	119	50	0.00%	0.001%
24	4.330	926	930	935	rVB2	200	218	0.02%	0.003%
25	4.372	940	943	945	rBV2	254	153	0.01%	0.002%
26	4.411	951	955	959	rBV	260	198	0.02%	0.002%
27	4.449	964	967	971	rVV	181	205	0.02%	0.002%
28	4.484	975	978	981	rBV2	223	162	0.01%	0.002%
29	4.520	985	989	990	rBV	200	80	0.01%	0.001%
30	4.552	997	999	1003	rBV	130	90	0.01%	0.001%
31	4.578	1004	1007	1008	rBV	178	109	0.01%	0.001%
32	4.616	1015	1019	1020	rBV2	210	137	0.01%	0.002%
33	4.668	1020	1035	1069	rBV	109643	258349	22.69%	3.144%
34	5.002	1134	1139	1141	rBV3	420	373	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU030320\
 Data File : VU037019.D
 Acq On : 03 Mar 2020 13:27
 Operator : JC/MD
 Sample : VU0303WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK37

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
 Title : VOC Analysis

35	5.105	1154	1171	1192	rBV	192888	426189	37.43%	5.187%
36	5.285	1223	1227	1230	rBV2	253	232	0.02%	0.003%
37	5.317	1233	1237	1238	rBV	433	268	0.02%	0.003%
38	5.378	1255	1256	1259	rBV	121	52	0.00%	0.001%
39	5.410	1259	1266	1267	rBV2	400	426	0.04%	0.005%
40	5.436	1272	1274	1276	rBV2	145	83	0.01%	0.001%
41	5.500	1291	1294	1299	rVB2	174	114	0.01%	0.001%
42	5.529	1299	1303	1306	rBV2	123	94	0.01%	0.001%
43	5.546	1306	1308	1310	rVV	159	84	0.01%	0.001%
44	5.603	1323	1326	1331	rVB2	201	177	0.02%	0.002%
45	5.629	1331	1334	1337	rBV	133	84	0.01%	0.001%
46	5.645	1337	1339	1341	rVB	141	37	0.00%	0.000%
47	5.671	1345	1347	1354	rVB	210	170	0.01%	0.002%
48	5.761	1354	1375	1401	rBV2	435694	1138719	100.00%	13.858%
49	6.144	1490	1494	1500	rVB3	377	332	0.03%	0.004%
50	6.282	1523	1537	1554	rBV	354031	661588	58.10%	8.052%
51	6.562	1615	1624	1631	rBV5	2639	4513	0.40%	0.055%
52	6.613	1637	1640	1642	rBV2	234	160	0.01%	0.002%
53	6.726	1660	1675	1697	rBV	266593	517921	45.48%	6.303%
54	6.893	1723	1727	1729	rVB	303	144	0.01%	0.002%
55	6.909	1729	1732	1734	rBV2	195	165	0.01%	0.002%
56	6.957	1744	1747	1750	rBV2	186	149	0.01%	0.002%
57	7.050	1773	1776	1778	rBV	216	146	0.01%	0.002%
58	7.079	1782	1785	1788	rBV2	150	119	0.01%	0.001%
59	7.124	1797	1799	1805	rVB2	309	296	0.03%	0.004%
60	7.160	1805	1810	1813	rBV	238	228	0.02%	0.003%
61	7.176	1813	1815	1817	rVV2	218	145	0.01%	0.002%
62	7.208	1819	1825	1835	rVV3	2494	4037	0.35%	0.049%
63	7.250	1835	1838	1841	rVB	194	98	0.01%	0.001%
64	7.262	1841	1842	1844	rVB	128	46	0.00%	0.001%
65	7.279	1844	1847	1850	rBV2	150	108	0.01%	0.001%
66	7.301	1851	1854	1857	rBV	128	90	0.01%	0.001%
67	7.491	1911	1913	1918	rVB	229	165	0.01%	0.002%
68	7.594	1932	1945	1960	rBV	139196	239335	21.02%	2.913%
69	7.790	1999	2006	2009	rBV	246	340	0.03%	0.004%
70	7.838	2018	2021	2024	rBV	169	165	0.01%	0.002%
71	7.925	2034	2048	2064	rBV	526815	897816	78.84%	10.926%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU030320\
 Data File : VU037019.D
 Acq On : 03 Mar 2020 13:27
 Operator : JC/MD
 Sample : VU0303WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK37

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
 Title : VOC Analysis

72	8.111	2103	2106	2112	rVB3	374	320	0.03%	0.004%
73	8.205	2123	2135	2153	rBV	98964	163277	14.34%	1.987%
74	8.398	2190	2195	2199	rBV2	304	393	0.03%	0.005%
75	8.430	2202	2205	2208	rVB2	273	164	0.01%	0.002%
76	8.452	2210	2212	2214	rBV	115	65	0.01%	0.001%
77	8.558	2241	2245	2249	rBV2	229	242	0.02%	0.003%
78	8.603	2257	2259	2261	rBV	160	84	0.01%	0.001%
79	8.661	2264	2277	2323	rVV	293429	546615	48.00%	6.652%
80	8.880	2342	2345	2351	rBV	256	273	0.02%	0.003%
81	8.986	2376	2378	2380	rBV	135	35	0.00%	0.000%
82	9.131	2421	2423	2429	rVB	238	149	0.01%	0.002%
83	9.198	2441	2444	2447	rBV	196	151	0.01%	0.002%
84	9.233	2453	2455	2457	rBV	155	67	0.01%	0.001%
85	9.314	2477	2480	2481	rBV	163	94	0.01%	0.001%
86	9.439	2506	2519	2556	rBV	493862	813752	71.46%	9.903%
87	9.709	2596	2603	2607	rBV2	346	399	0.04%	0.005%
88	9.825	2635	2639	2641	rBV2	249	198	0.02%	0.002%
89	9.899	2658	2662	2665	rBV2	277	221	0.02%	0.003%
90	9.928	2665	2671	2673	rBV2	249	272	0.02%	0.003%
91	10.169	2745	2746	2747	rVB	474	91	0.01%	0.001%
92	10.777	2923	2935	2951	rVB	335167	539652	47.39%	6.568%
93	11.005	3001	3006	3009	rBV2	255	294	0.03%	0.004%
94	11.060	3020	3023	3025	rBV2	189	116	0.01%	0.001%
95	11.378	3119	3122	3125	rBV	290	250	0.02%	0.003%
96	11.436	3136	3140	3143	rBV	250	242	0.02%	0.003%
97	11.831	3250	3263	3279	rBV	366798	607304	53.33%	7.391%
98	12.211	3368	3381	3399	rVB	396173	652638	57.31%	7.943%
99	12.706	3532	3535	3539	rBV	406	397	0.03%	0.005%
100	12.799	3562	3564	3565	rBV	254	85	0.01%	0.001%


Sum of corrected areas: 8216918

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU030320\
Data File : VU037019.D
Acq On : 03 Mar 2020 13:27
Operator : JC/MD
Sample : VU0303WBL01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK37

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

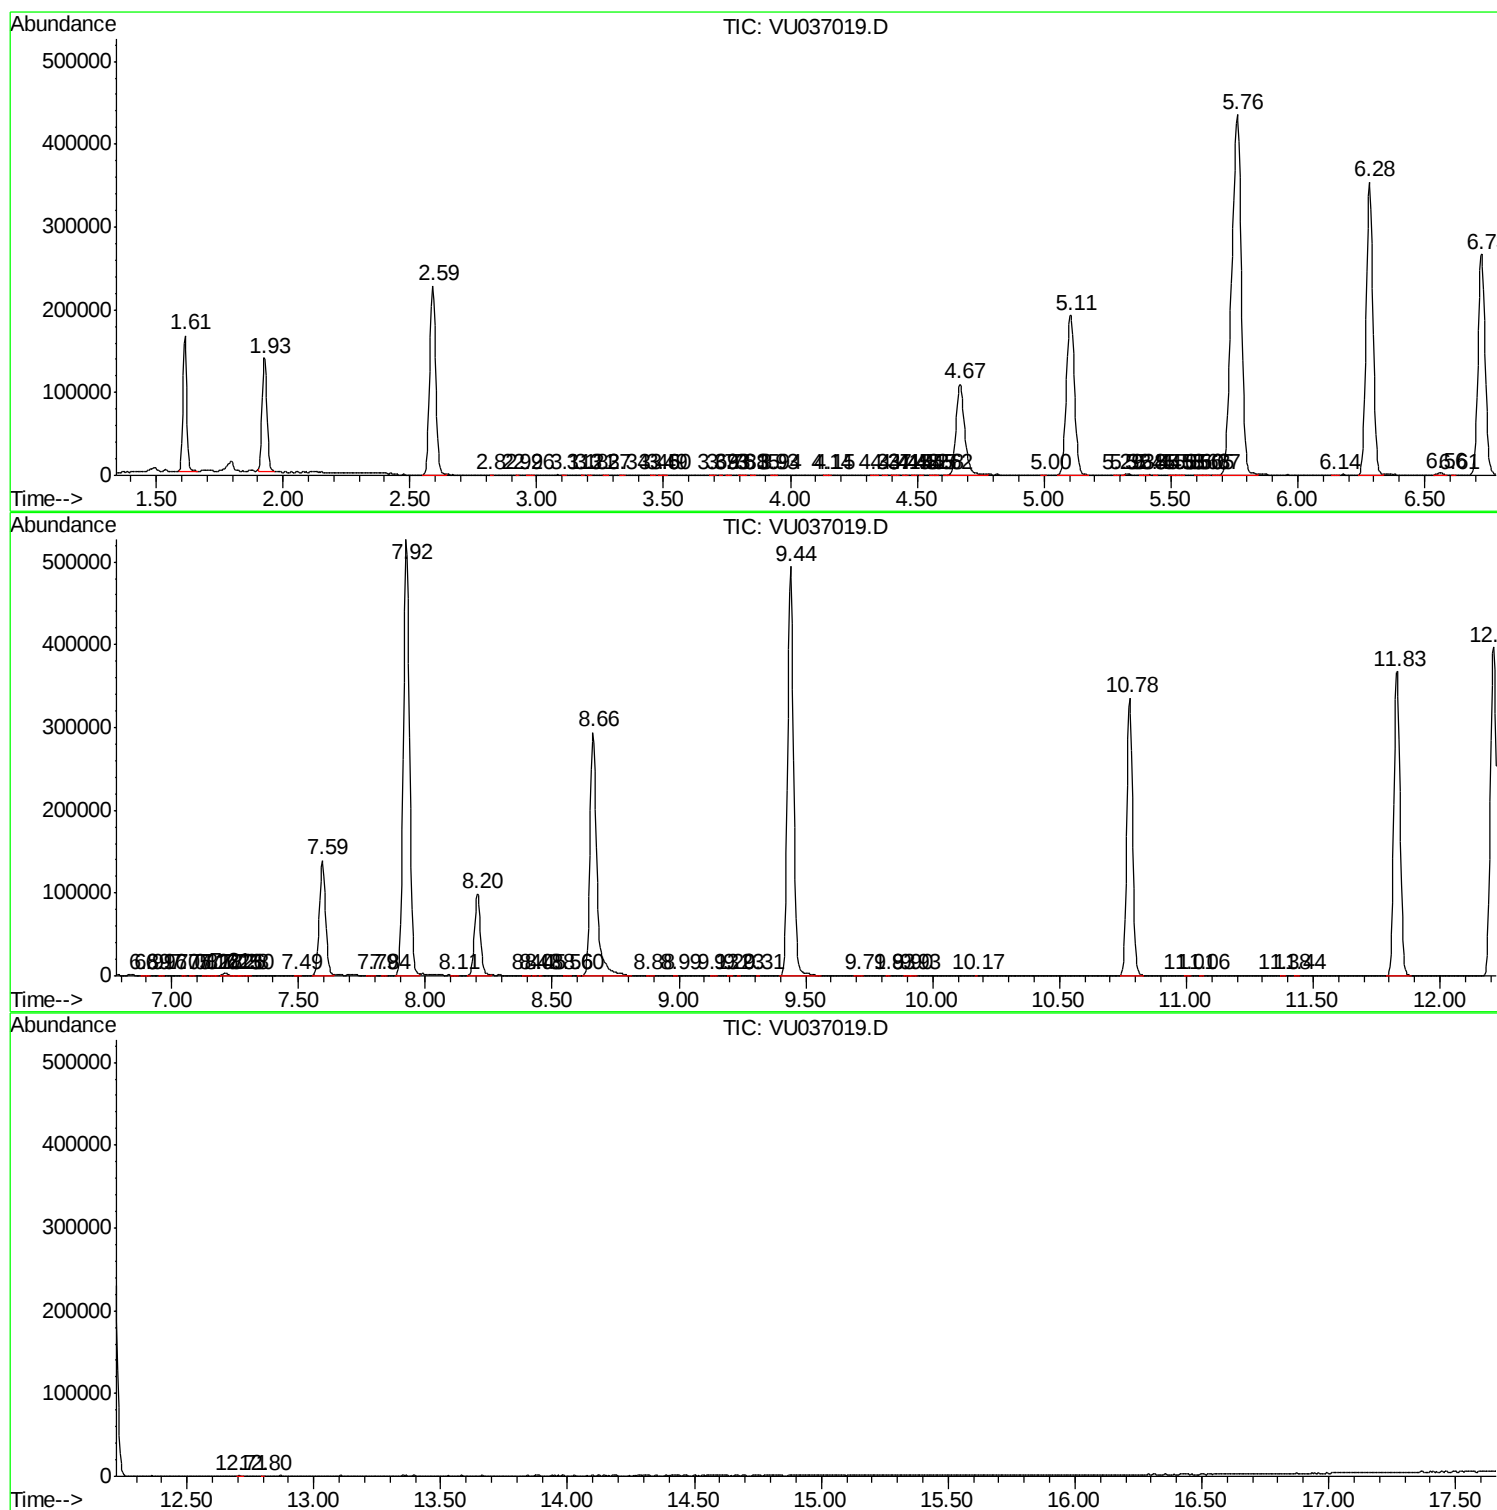

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU030320\
Data File : VU037019.D
Acq On : 03 Mar 2020 13:27
Operator : JC/MD
Sample : VU0303WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK37

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU030320\
Data File : VU037019.D
Acq On : 03 Mar 2020 13:27
Operator : JC/MD
Sample : VU0303WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK37

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc