


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU030320\
 Data File : VU037017.D
 Acq On : 03 Mar 2020 10:33
 Operator : JC/MD
 Sample : BFB56
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB56

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM022420WMA.M
 Title : VOC Analysis
 Last Update : Thu Mar 05 02:52:45 2020

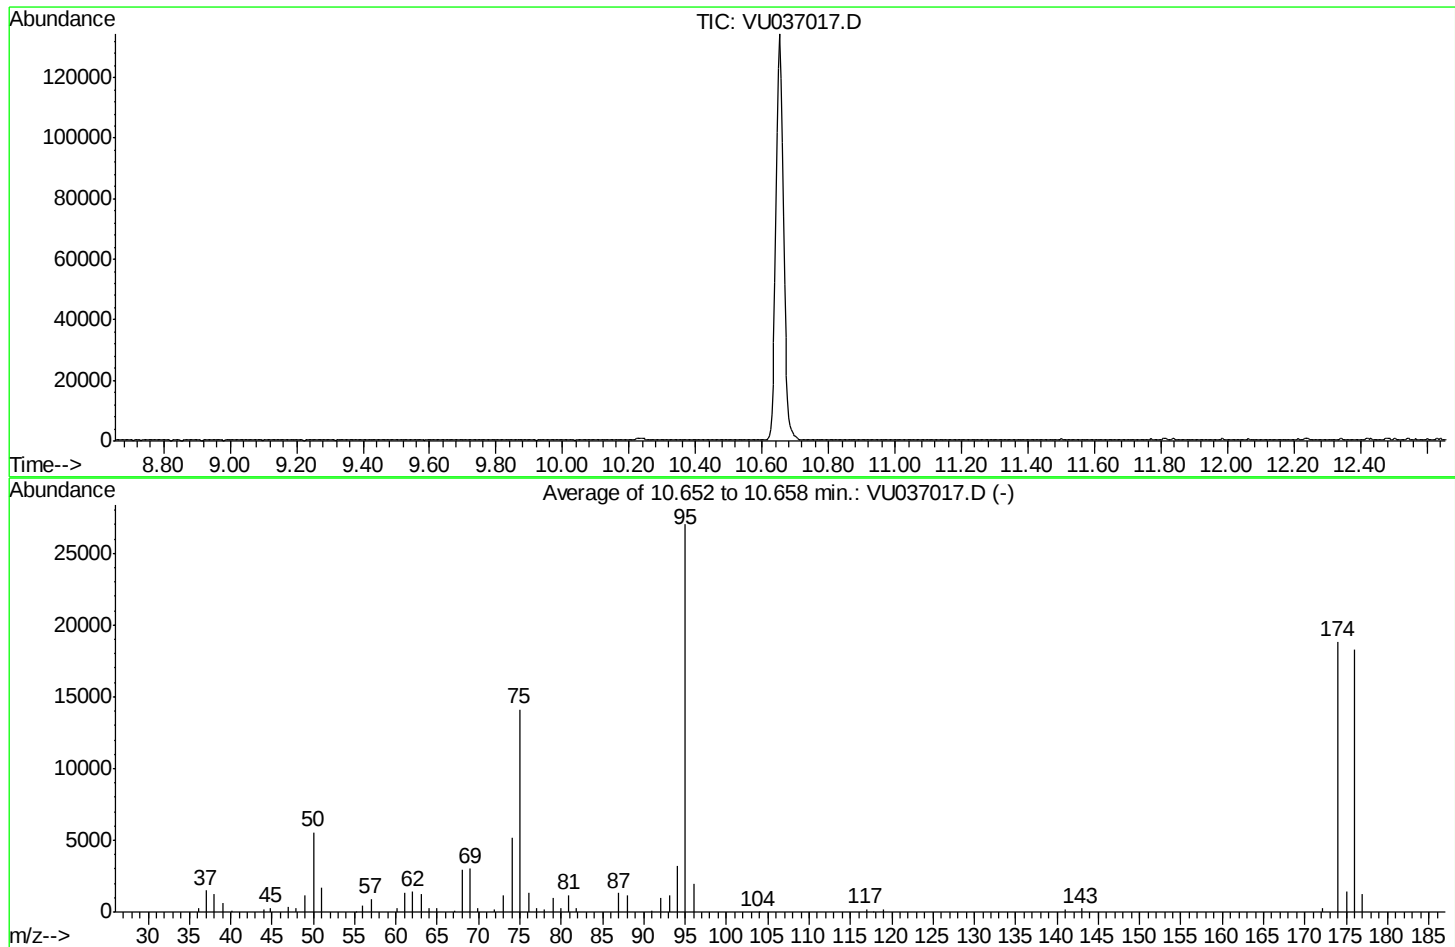

AutoFind: Scans 2896, 2897, 2898; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	5535	PASS
75	95	30	80	52.2	14103	PASS
95	95	100	100	100.0	27021	PASS
96	95	5	9	7.1	1929	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	69.7	18829	PASS
175	174	5	9	7.8	1471	PASS
176	174	95	101	97.2	18296	PASS
177	176	5	9	7.0	1284	PASS

m/z	Abundance
36.00	339.0
37.00	1670.0
38.00	1363.0
39.00	608.0
39.90	114.0
44.00	527.0
44.90	323.0
46.90	350.0
47.80	266.0
49.00	1256.0
50.00	5938.0
51.00	1814.0
55.20	103.0
56.00	509.0
57.00	919.0
60.10	310.0
61.00	1407.0
62.00	1462.0
63.00	1294.0
64.00	207.0
65.00	265.0
67.10	106.0
68.00	3157.0
69.00	3114.0
70.00	308.0
71.90	178.0
73.00	1222.0
74.10	5148.0
75.00	14970.0
76.00	1341.0
76.90	274.0
78.00	190.0
78.90	1000.0
79.90	298.0
80.90	1313.0
81.90	260.0
87.00	1397.0
88.00	1280.0
92.00	978.0
93.00	1187.0
94.10	3386.0
95.00	27840.0
96.00	2092.0
103.90	106.0
116.90	190.0
117.80	106.0
119.00	206.0
140.90	251.0
142.90	273.0
172.00	267.0
174.00	19272.0
175.10	1484.0
176.00	18832.0
177.00	1295.0

Instrument :
MSVOA_U
ClientSampleId :
BFB56

m/z	Abundance
36.10	326.0
37.00	1547.0
38.00	1295.0
39.00	631.0
40.10	142.0
44.00	493.0
44.90	306.0
46.90	341.0
47.90	269.0
49.00	1217.0
50.00	5661.0
51.00	1726.0
56.00	473.0
57.00	929.0
60.00	298.0
61.00	1397.0
62.00	1421.0
63.00	1305.0
64.00	237.0
65.00	290.0
67.00	108.0
68.00	3031.0
69.00	3083.0
69.90	312.0
71.80	164.0
73.00	1225.0
74.00	5269.0
75.00	14387.0
76.00	1382.0
77.00	251.0
78.00	213.0
79.00	956.0
80.00	254.0
80.90	1259.0
81.90	271.0
86.90	1364.0
88.00	1177.0
90.90	117.0
92.00	997.0
93.10	1213.0
94.10	3270.0
95.00	27984.0
96.00	1993.0
116.90	207.0
119.00	213.0
141.00	223.0
143.00	268.0
172.00	264.0
174.00	19440.0
175.10	1533.0
176.00	18856.0
177.00	1319.0

Instrument :
MSVOA_U
ClientSampleId :
BFB56

m/z	Abundance
36.00	263.0
37.00	1304.0
38.00	1058.0
39.00	560.0
40.10	152.0
44.00	468.0
44.80	267.0
46.90	280.0
47.90	238.0
48.90	1086.0
50.00	5006.0
51.00	1434.0
56.00	404.0
57.00	846.0
60.00	241.0
61.00	1305.0
62.00	1295.0
63.00	1166.0
64.10	239.0
65.00	294.0
68.00	2672.0
69.00	2785.0
69.90	256.0
71.80	130.0
73.00	1087.0
74.00	5014.0
75.00	12952.0
76.10	1222.0
77.10	202.0
78.00	183.0
79.00	881.0
80.00	214.0
80.90	1014.0
81.80	241.0
86.90	1193.0
88.00	1011.0
90.90	121.0
92.00	917.0
93.00	1126.0
94.10	2954.0
95.00	25240.0
96.00	1704.0
116.90	207.0
119.00	178.0
141.00	171.0
143.00	242.0
172.10	247.0
174.00	17776.0
175.00	1398.0
176.00	17200.0
177.00	1240.0

Instrument :
MSVOA_U
ClientSampleId :
BFB56

Scan 2884 (10.613 min): VU037017.D
BFB56

m/z	Abundance
39.90	149.0
43.90	271.0

Instrument :
MSVOA_U
ClientSampleId :
BFB56