

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU030419\
 Data File : VU029790.D
 Acq On : 04 Mar 2019 18:03
 Operator : JC/SP
 Sample : K1661-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC70

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM021519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	24	29	36	rVB2	7077	6891	0.49%	0.057%
2	1.396	88	95	109	rBV	213793	218640	15.49%	1.811%
3	1.679	175	183	196	rVB	162721	202317	14.33%	1.676%
4	2.270	356	367	379	rBV	333823	506941	35.91%	4.199%
5	2.405	403	409	414	rVB4	624	755	0.05%	0.006%
6	2.444	417	421	423	rBV2	921	623	0.04%	0.005%
7	2.592	464	467	469	rBV2	467	333	0.02%	0.003%
8	2.637	478	481	484	rBV2	582	411	0.03%	0.003%
9	2.701	496	501	507	rBV3	751	967	0.07%	0.008%
10	2.804	529	533	535	rBV2	641	472	0.03%	0.004%
11	2.833	535	542	552	rVB5	1779	3147	0.22%	0.026%
12	2.987	586	590	595	rVB3	463	485	0.03%	0.004%
13	3.074	614	617	619	rBV	503	346	0.02%	0.003%
14	3.177	642	649	653	rBV2	555	537	0.04%	0.004%
15	3.383	707	713	716	rBV2	437	359	0.03%	0.003%
16	3.617	778	786	790	rBV3	649	849	0.06%	0.007%
17	3.640	790	793	798	rVB3	442	399	0.03%	0.003%
18	3.714	812	816	819	rBV	394	357	0.03%	0.003%
19	3.836	849	854	855	rBV	430	332	0.02%	0.003%
20	3.881	864	868	871	rBV2	382	342	0.02%	0.003%
21	3.987	896	901	905	rVB2	559	512	0.04%	0.004%
22	4.039	912	917	922	rVB3	505	576	0.04%	0.005%
23	4.174	946	959	991	rBV	150862	403950	28.61%	3.346%
24	4.431	1035	1039	1042	rBV2	786	717	0.05%	0.006%
25	4.476	1050	1053	1056	rVB2	549	352	0.02%	0.003%
26	4.646	1089	1106	1135	rBV	229172	546768	38.73%	4.529%
27	4.887	1171	1181	1192	rVB4	1053	1933	0.14%	0.016%
28	5.026	1220	1224	1228	rBV2	440	409	0.03%	0.003%
29	5.058	1230	1234	1237	rBV	446	384	0.03%	0.003%
30	5.248	1287	1293	1297	rBV2	348	358	0.03%	0.003%
31	5.338	1297	1321	1351	rBV2	486451	1411829	100.00%	11.693%
32	5.575	1392	1395	1398	rVB3	554	435	0.03%	0.004%
33	5.659	1415	1421	1423	rBV3	525	595	0.04%	0.005%
34	5.691	1428	1431	1434	rBV2	397	355	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU030419\
 Data File : VU029790.D
 Acq On : 04 Mar 2019 18:03
 Operator : JC/SP
 Sample : K1661-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC70

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM021519WMA.M
 Title : VOC Analysis

35	5.756	1444	1451	1457	rVB4	977	1491	0.11%	0.012%
36	5.797	1457	1464	1467	rBV2	862	1070	0.08%	0.009%
37	5.817	1467	1470	1474	rVB2	495	347	0.02%	0.003%
38	5.884	1474	1491	1517	rBV	541893	1065334	75.46%	8.824%
39	6.090	1552	1555	1560	rVV3	433	354	0.03%	0.003%
40	6.129	1563	1567	1570	rVB3	513	395	0.03%	0.003%
41	6.174	1574	1581	1584	rBV5	2283	3089	0.22%	0.026%
42	6.328	1615	1629	1658	rBV	307715	619698	43.89%	5.133%
43	6.637	1721	1725	1731	rVB2	557	548	0.04%	0.005%
44	6.669	1731	1735	1738	rBV3	571	504	0.04%	0.004%
45	6.762	1760	1764	1767	rBV3	468	369	0.03%	0.003%
46	6.794	1772	1774	1780	rBV2	469	407	0.03%	0.003%
47	6.846	1787	1790	1792	rBV	534	373	0.03%	0.003%
48	7.003	1834	1839	1843	rVB3	718	763	0.05%	0.006%
49	7.064	1854	1858	1863	rBV2	737	617	0.04%	0.005%
50	7.145	1878	1883	1888	rVB3	306	395	0.03%	0.003%
51	7.225	1896	1908	1933	rBV	171579	312539	22.14%	2.589%
52	7.415	1964	1967	1970	rBV3	578	447	0.03%	0.004%
53	7.508	1992	1996	2000	rVB2	679	584	0.04%	0.005%
54	7.563	2000	2013	2034	rBV	675651	1180274	83.60%	9.776%
55	7.846	2091	2101	2124	rBV	117795	207014	14.66%	1.715%
56	8.096	2176	2179	2182	rBV	587	488	0.03%	0.004%
57	8.177	2194	2204	2212	rVB3	6342	10597	0.75%	0.088%
58	8.222	2215	2218	2226	rVB3	674	657	0.05%	0.005%
59	8.309	2233	2245	2278	rBV	553524	1005095	71.19%	8.325%
60	8.710	2366	2370	2374	rVB3	589	489	0.03%	0.004%
61	8.755	2381	2384	2390	rVB2	695	696	0.05%	0.006%
62	8.794	2390	2396	2397	rBV2	686	607	0.04%	0.005%
63	8.952	2439	2445	2448	rBV2	476	437	0.03%	0.004%
64	9.013	2459	2464	2470	rVB3	679	741	0.05%	0.006%
65	9.087	2474	2487	2527	rBV	777106	1306311	92.53%	10.820%
66	9.376	2572	2577	2581	rBV3	552	537	0.04%	0.004%
67	9.485	2607	2611	2614	rVV3	418	369	0.03%	0.003%
68	9.566	2633	2636	2641	rVB2	493	368	0.03%	0.003%
69	9.733	2685	2688	2692	rVB3	525	341	0.02%	0.003%
70	9.823	2714	2716	2723	rVB	696	738	0.05%	0.006%
71	9.990	2765	2768	2770	rBV2	739	569	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU030419\
 Data File : VU029790.D
 Acq On : 04 Mar 2019 18:03
 Operator : JC/SP
 Sample : K1661-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC70

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM021519WMA.M
 Title : VOC Analysis

72	10.212	2833	2837	2842	rBV2	444	503	0.04%	0.004%
73	10.427	2890	2904	2930	rBV	486724	788458	55.85%	6.530%
74	10.604	2951	2959	2970	rVV4	4885	8115	0.57%	0.067%
75	10.762	3003	3008	3011	rVB	362	394	0.03%	0.003%
76	10.804	3017	3021	3025	rVV2	524	503	0.04%	0.004%
77	10.833	3025	3030	3033	rVV3	639	660	0.05%	0.005%
78	10.881	3042	3045	3047	rVV2	500	365	0.03%	0.003%
79	10.894	3047	3049	3053	rVB2	632	431	0.03%	0.004%
80	10.951	3064	3067	3072	rBV2	498	431	0.03%	0.004%
81	11.000	3079	3082	3089	rVB2	458	385	0.03%	0.003%
82	11.218	3147	3150	3153	rBV	646	496	0.04%	0.004%
83	11.421	3205	3213	3217	rBV5	884	1041	0.07%	0.009%
84	11.482	3217	3232	3258	rBV	733264	1174137	83.16%	9.725%
85	11.717	3301	3305	3310	rVB3	928	887	0.06%	0.007%
86	11.768	3310	3321	3326	rBV6	3268	6658	0.47%	0.055%
87	11.858	3336	3349	3367	rBV	636770	1041536	73.77%	8.627%
88	12.279	3477	3480	3483	rBV3	655	339	0.02%	0.003%
89	12.328	3492	3495	3499	rVB3	692	453	0.03%	0.004%
90	12.353	3499	3503	3507	rBV2	622	623	0.04%	0.005%
91	12.479	3535	3542	3548	rBV4	1260	1924	0.14%	0.016%
92	12.627	3585	3588	3594	rVB2	494	538	0.04%	0.004%
93	12.823	3646	3649	3652	rBV2	1037	728	0.05%	0.006%
94	12.903	3671	3674	3677	rBV2	563	389	0.03%	0.003%
95	13.035	3713	3715	3720	rVB	623	335	0.02%	0.003%
96	13.279	3789	3791	3798	rVB3	773	815	0.06%	0.007%
97	13.315	3799	3802	3805	rBV2	559	388	0.03%	0.003%
98	13.675	3911	3914	3919	rVB3	796	652	0.05%	0.005%
99	14.260	4093	4096	4098	rBV2	659	412	0.03%	0.003%
100	14.768	4251	4254	4257	rBV3	984	699	0.05%	0.006%


Sum of corrected areas: 12073623

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU030419\
Data File : VU029790.D
Acq On : 04 Mar 2019 18:03
Operator : JC/SP
Sample : K1661-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC70

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM021519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

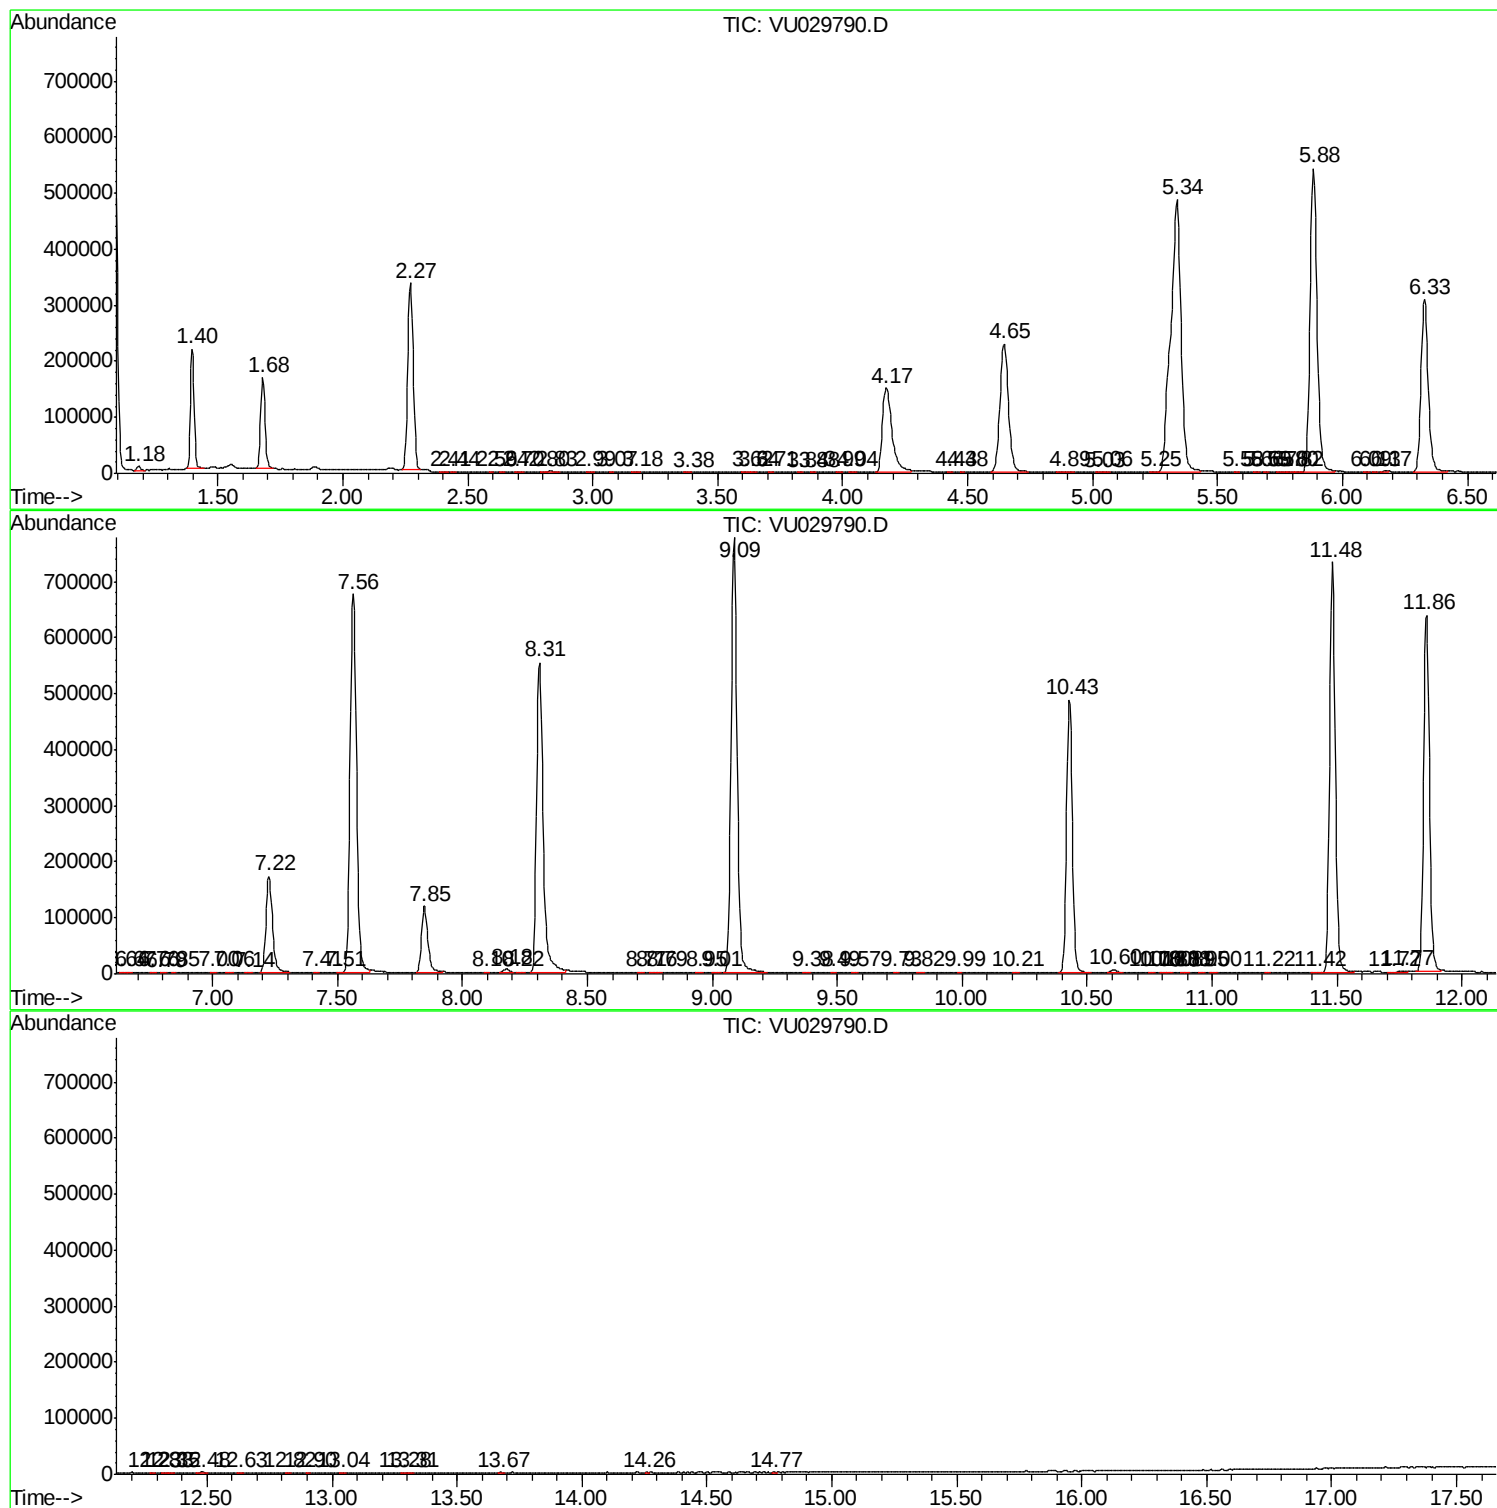

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU030419\
Data File : VU029790.D
Acq On : 04 Mar 2019 18:03
Operator : JC/SP
Sample : K1661-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC70

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM021519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU030419\
Data File : VU029790.D
Acq On : 04 Mar 2019 18:03
Operator : JC/SP
Sample : K1661-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC70

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM021519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc