


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030419\
Data File : VU029772.D
Acq On : 04 Mar 2019 09:08
Operator : JC/SP
Sample : BFB54
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB54

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM021519WMA.M
Title : VOC Analysis
Last Update : Tue Mar 05 01:28:42 2019

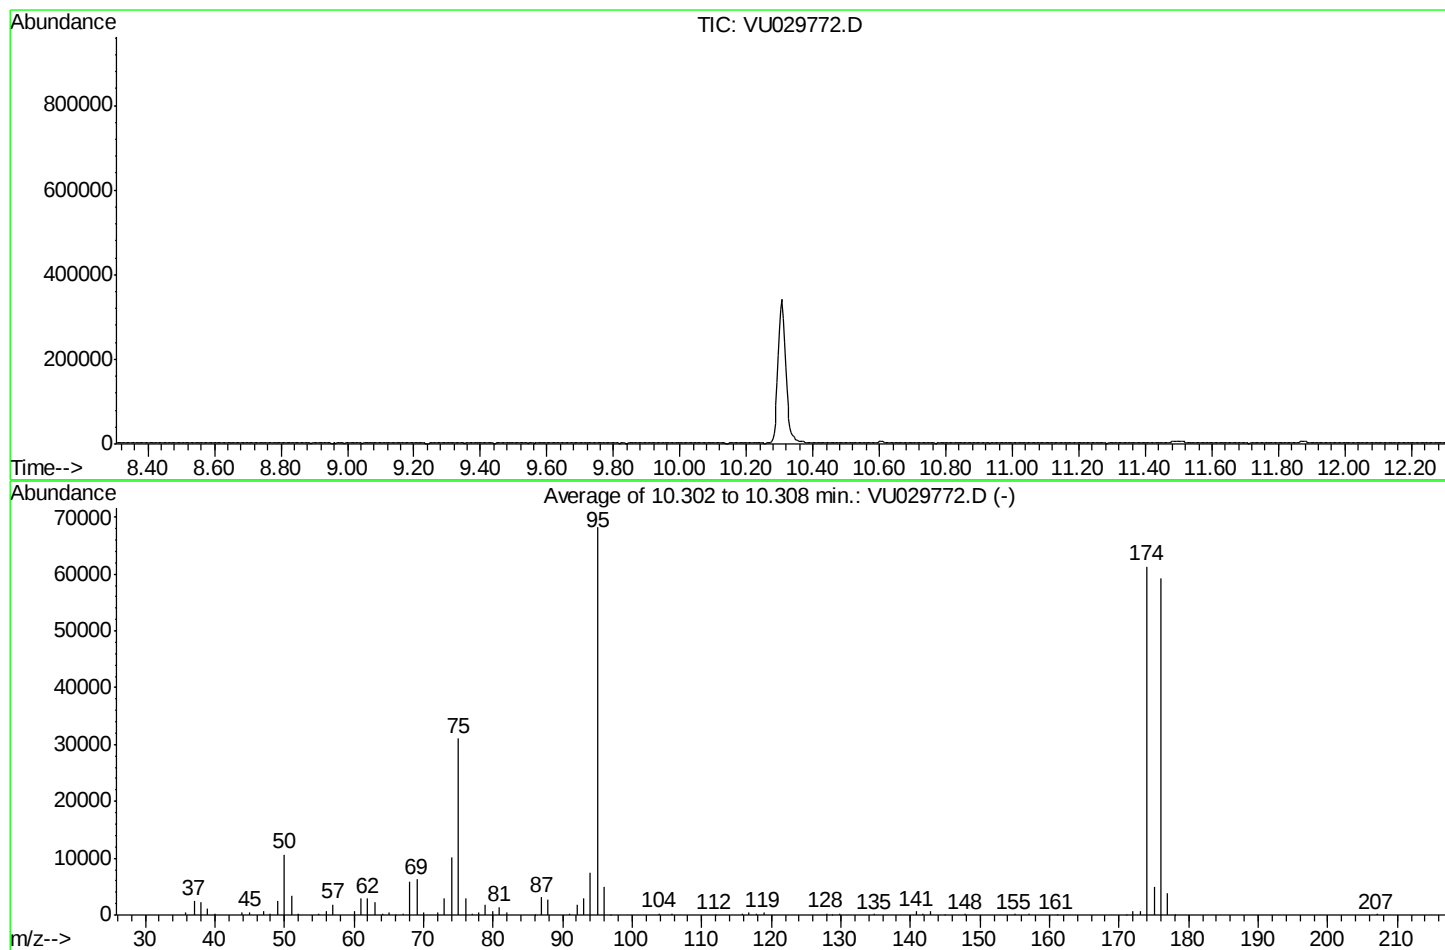

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	10684	PASS
75	95	30	80	45.5	31069	PASS
95	95	100	100	100.0	68213	PASS
96	95	5	9	7.2	4937	PASS
173	174	0.00	2	1.1	703	PASS
174	95	50	120	90.0	61365	PASS
175	174	5	9	7.9	4873	PASS
176	174	95	101	96.7	59338	PASS
177	176	5	9	6.4	3797	PASS

m/z	Abundance
35.90	339.0
37.00	2537.0
38.00	2180.0
39.00	1114.0
40.00	1685.0
44.00	781.0
45.00	498.0
47.00	776.0
47.90	274.0
49.00	2504.0
50.00	10462.0
51.00	3269.0
52.10	130.0
54.90	207.0
56.00	768.0
57.00	1880.0
60.00	618.0
61.00	2766.0
62.00	2858.0
63.00	2288.0
64.00	302.0
65.00	458.0
67.00	166.0
68.00	5736.0
69.00	6369.0
70.00	434.0
72.00	360.0
73.00	2768.0
74.00	9902.0
75.00	30280.0
76.00	2874.0
77.00	368.0
77.90	360.0
78.90	1946.0
79.90	659.0
81.00	1284.0
81.90	471.0
87.00	2973.0
87.90	2565.0
91.00	154.0
92.10	1839.0
93.00	2903.0
94.00	7346.0
95.10	65480.0
96.00	4847.0
97.00	100.0
103.90	247.0
105.80	172.0
115.80	210.0
116.80	373.0
117.90	249.0
118.90	356.0
127.90	216.0
129.90	227.0
134.80	209.0
140.90	541.0
141.80	103.0
142.90	535.0
144.90	101.0
148.00	126.0
155.00	176.0
157.00	111.0
171.10	109.0
172.00	664.0
173.10	663.0
174.00	58272.0
175.00	4567.0
176.00	56016.0
177.00	3513.0
178.00	144.0
207.10	158.0

Instrument :
MSVOA_U
ClientSampleId :
BFB54

m/z	Abundance
35.80	361.0
37.00	2618.0
38.00	2244.0
39.00	1119.0
40.00	1584.0
43.90	720.0
45.00	545.0
47.00	723.0
47.90	276.0
49.00	2576.0
50.00	11079.0
51.00	3532.0
52.00	139.0
54.90	223.0
56.00	769.0
57.00	1985.0
60.00	747.0
61.00	2944.0
62.00	3014.0
63.00	2291.0
64.10	322.0
65.10	497.0
67.00	209.0
68.00	6048.0
69.00	6468.0
70.10	449.0
71.90	373.0
73.00	2927.0
74.00	10428.0
75.00	32200.0
76.10	3080.0
76.90	328.0
77.90	392.0
78.90	1896.0
79.90	685.0
80.90	1492.0
81.90	500.0
86.00	102.0
87.00	3277.0
88.00	2824.0
90.90	185.0
92.00	1808.0
93.00	2920.0
94.00	7730.0
95.10	70792.0
96.00	5073.0
97.00	102.0
103.90	296.0
105.80	205.0
115.80	151.0
116.80	377.0
117.90	286.0
118.90	379.0
127.90	237.0
128.80	100.0
129.90	218.0
134.80	200.0
140.90	627.0
141.70	141.0
142.90	581.0
144.90	103.0
147.90	134.0
155.00	194.0
157.00	148.0
161.10	102.0
172.00	721.0
173.10	735.0
174.00	63176.0
175.00	5058.0
176.00	61288.0
177.00	3907.0
178.00	136.0
207.00	141.0

Instrument :
MSVOA_U
ClientSampleId :
BFB54

m/z	Abundance
35.80	379.0
37.00	2544.0
38.00	2129.0
39.00	1037.0
40.00	1486.0
43.90	603.0
45.00	500.0
47.10	651.0
48.00	310.0
49.00	2470.0
50.00	10513.0
51.00	3609.0
52.00	140.0
55.00	203.0
56.00	762.0
57.00	1859.0
60.00	708.0
61.00	2863.0
62.00	2718.0
63.00	2187.0
64.10	344.0
65.10	494.0
65.90	126.0
67.00	237.0
68.00	6073.0
69.00	6072.0
70.10	441.0
71.90	334.0
73.00	2788.0
74.00	9914.0
75.00	30728.0
76.10	3008.0
77.00	285.0
78.00	360.0
78.90	1749.0
80.00	608.0
80.90	1639.0
82.00	498.0
87.00	3026.0
88.00	2791.0
90.90	223.0
92.00	1850.0
93.00	2706.0
94.00	7548.0
95.00	68368.0
96.00	4892.0
96.90	124.0
103.90	289.0
105.80	193.0
111.90	105.0
115.80	120.0
116.80	308.0
117.90	284.0
118.90	409.0
127.90	234.0
128.80	102.0
129.80	211.0
134.80	172.0
140.90	603.0
141.70	129.0
142.90	608.0
144.80	104.0
147.80	142.0
155.00	185.0
157.00	158.0
161.00	100.0
172.00	716.0
173.10	711.0
174.00	62648.0
175.00	4994.0
176.00	60712.0
177.00	3972.0
207.00	135.0

Instrument :
MSVOA_U
ClientSampleId :
BFB54

m/z	Abundance
39.90	1333.0
41.00	117.0
44.00	349.0

Instrument :
MSVOA_U
ClientSampleId :
BFB54